

RANDOX

RANDOX INTERNATIONAL
QUALITY ASSESSMENT SCHEME



RIQAS

RANDOX

QUALITY CONTROL

RIQAS

THE LARGEST INTERNATIONAL EQA SCHEME
WITH OVER 45,000 LAB PARTICIPANTS



01	BENEFITS
02	EQA
03	RIQAS REPORTS
04	WEB-BASED DATA TRANSFER
05	PARTICIPATION IN RIQAS
06	STANDARD REPORT
07	TEXT SECTION
08	HISTOGRAM
09	LEVEY-JENNINGS CHART
10	TARGET SCORE CHART
11	%DEVIATION CHARTS
12	MULTI-METHOD STAT SECTION
13	SUMMARY PAGE
14	MULTI-INSTRUMENT REPORT
15	URINE TOXICOLOGY REPORT
16	URINE TOXICOLOGY REPORT SCREENING SECTION
17	URINE TOXICOLOGY REPORT QUANTITATIVE SECTION
18	URINALYSIS REPORT
19	SEROLOGY: SCREENING (QUALITATIVE) REPORT
20	SEROLOGY: SCREENING (QUANTITATIVE) REPORT
21	QUANTITATIVE END-OF-CYCLE REPORT
22	CHART SECTION (END-OF-CYCLE REPORT)
23	TEXT SECTION (END-OF-CYCLE REPORT)
25	CURRENT & PREVIOUS CYCLE ABSOLUTE SDIs (END-OF-CYCLE REPORT)
26	CERTIFICATE OF PERFORMANCE (END-OF-CYCLE REPORT)
27	MONITORING EQA PERFORMANCE
30	RIQAS PROGRAMMES
35	PARAMETER INDEX
49	RELATED PRODUCTS
51	RANDOX - A GLOBAL DIAGNOSTIC SOLUTIONS PROVIDER
52	CONTACT US

BENEFITS

Delivering a comprehensive yet cost effective EQA solution, RIQAS will help meet regulatory requirements and increase confidence in test system accuracy.



Large Database of Users

- A high level of participation means peer group numbers are maximised whilst ensuring availability of data for a wide range of instruments and methods.



User-friendly Reports

- Simple, one page per parameter format, enables at-a-glance performance assessment, saving valuable laboratory time.
- Complimentary multi-instrument and interlaboratory reports allow comparative performance assessment of all laboratory systems and multiple connected laboratories.
- End-of-Cycle reports, summarising performance compared to the previous cycle, allow you to identify improvements in quality over time.



Cost Effective

- Our extensive range of multi-analyte programmes will reduce the number of individual programmes required to cover your test menu, saving both time and money.
- Reduced parameter options for selected programmes offer greater flexibility, ensuring suitability for laboratories of all sizes and budgets.
- Register up to five instruments per programme (volume permitting) at no extra cost for comparative performance assessment.



Frequency

- Frequent reporting allows early identification of system errors and implementation of any necessary corrective actions with minimum disruption to the lab.
- With a turnaround of less than 72 hours for most reports, corrective action can be implemented earlier, potentially reducing costly errors with patient results.



High Quality Samples

- Samples spanning clinically relevant levels allow identification of concentration related biases, helping to ensure accurate instrument performance.
- Human samples free from interfering preservatives increase confidence that EQA performance mirrors the performance of patient samples.
- Reference method values are provided in the Clinical Chemistry programme for selected parameters and lots while for the Immunosuppressant programme they are provided for all parameters and lots.




Highly Accredited

- Programmes accepted by National and International accreditation bodies worldwide.
- Participant certificates provide evidence of participation in a reputable EQA scheme.

RIQAS is the largest international EQA scheme in the world. It is used by more than 45,000 laboratory participants in 133 countries. 33 programmes are currently available.

RIQAS Programmes

- Ammonia/Ethanol
- Anti-TSH Receptor
- Blood Gas
- BNP
- Cardiac
- Cerebrospinal Fluid (CSF)
- Clinical Chemistry
- Coagulation
- CO-Oximetry
- CYFRA 21-I
- ESR
- Glycated Haemoglobin (HbA1c)
- Haematology
- Human Urine
- Immunoassay
- Immunoassay Speciality 1
- Immunoassay Speciality 2
- Immunosuppressant Drugs
- Lipid
- Liquid Cardiac
- Maternal Screening
- Serology Epstein Barr Virus (EBV)
- Serology (HIV/Hepatitis)
- Serology (Syphilis)
- Serology (ToRCH)
- Specific Proteins
- Sweat Testing
- Therapeutic Drugs
- Trace Elements in Blood
- Trace Elements in Serum
- Trace Elements in Urine
- Urinalysis
- Urine Toxicology

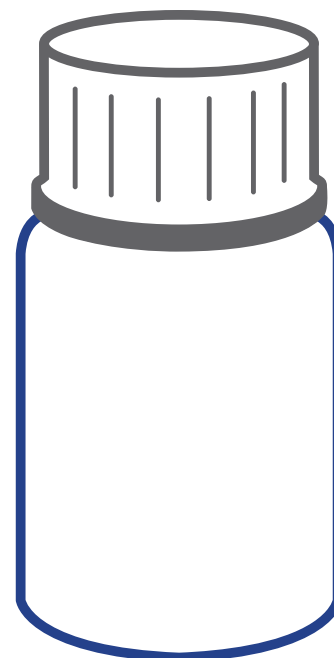

Accreditation

- RIQAS provides certificates as proof of EQA participation and performance for laboratory accreditation purposes.
- RIQAS is a UKAS accredited Proficiency Testing Provider, No. 0010, and is accredited to ISO/IEC 17043:2010, 'Conformity Assessment- General Requirements for Proficiency Testing'.
- Accreditation to ISO/IEC 17043:2010 highlights the superior quality and excellence of RIQAS.

UK Performance Surveillance

- Recognised by the Joint Working Group on Quality Assurance (JWG QA).
- Recognised by various National Quality Assurance Advisory Panels (NQAAP).

Independent Advisory Panel

RIQAS participants have access to an independent advisory panel consisting of scientific and clinical experts. This ensures professional and ethical conduct of the scheme and participant confidentiality.


 RIQAS support staff are on hand to offer
 advice and troubleshoot technical queries.

RIQAS REPORTS

RIQAS reports are presented in a user-friendly, one page per parameter format. This allows easy interpretation of your analytical performance.

RIQAS Reports

- Statistical breakdown by all methods, your method and, where applicable, your instrument, including running means for the last 10 samples.
- Compare your instrument group, method group and all methods using the histogram.
- Identify trends, biases and precision problems using the visual charts.
- The Target Score chart grades your performance in a moving window over the last 20 samples, including the previous cycle.
- At-a-glance summary page for all parameters in the programme.
- Compare your result with statistically robust consensus means.
- Identify acceptable and poor performance using fit-for-purpose performance indicators:
 - SDI
 - %Deviation
 - Target Score

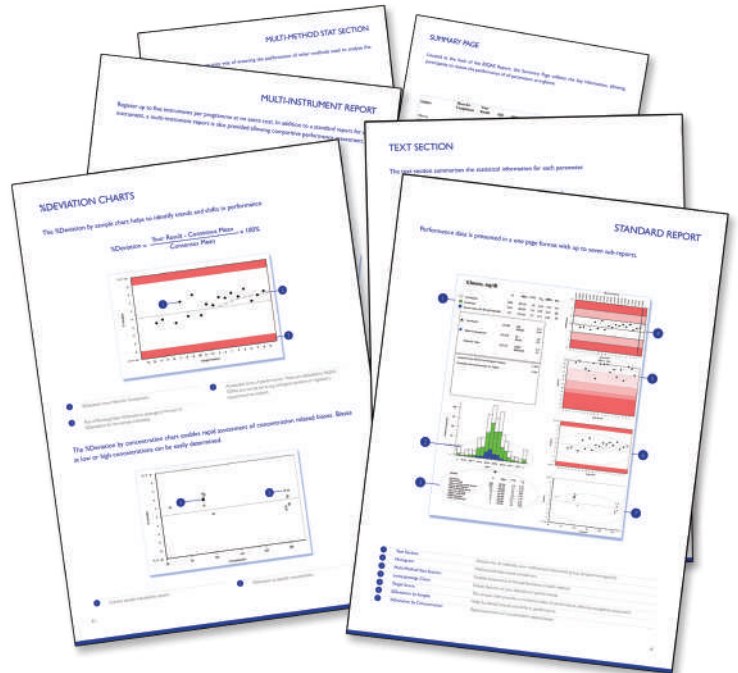

Summary CSV Files

It is possible to receive an additional summary of your report statistics, acceptable limits and performance indicators as a .csv file for every sample.

Multi-Instrument Reports

Laboratories can register up to five instruments at no extra cost. Individual reports for each instrument plus a unique multi-instrument report are provided. The multi-instrument report plots the performance of each individual instrument on a single, colour coded Levey-Jennings chart, ensuring instant identification of any differences in instrument performance. Additional sample packs may be ordered as required if volume supplied is insufficient for the registered instruments.



Laboratory Group Reports

The Group Reporting facility enables laboratory groups or chains to monitor the performance of satellite sites. Each affiliated laboratory will receive their individual reports with the group supervisor also receiving a summary report comparing each laboratory in the network.

WEB-BASED DATA TRANSFER

RIQAS.Net offers easy, direct access for the submission of results and retrieval of reports direct from the RIQAS host server.

- Available in multiple languages.
- Confidentiality and security is maintained through the use of password protected access.
- Submit current, corrected and future results (normal policies apply), directly into the RIQAS database. Receipt of results is confirmed by e-mail.
- Multi-lingual registration identifier provides simple identification of multiple registrations.
- Additions and changes to assay details can be made quickly and easily online.
- Requests for new method, instrument and reagent codes can be made online.
- Reports are emailed in PDF format as soon as they are prepared.
- Reports for the previous two cycles can be downloaded from the website.
- View, print, store or distribute reports as you wish.
- Update your laboratory's certificate of participation details in multiple languages.
- All that is required is web access, Adobe Reader (for viewing reports) and a valid password to access the system.
- No additional software required.

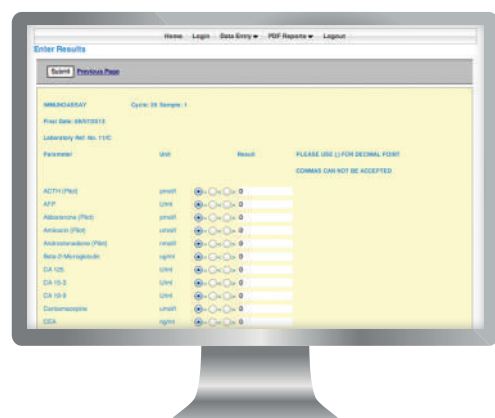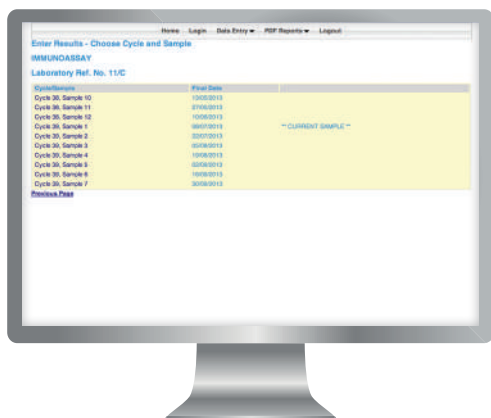


PARTICIPATION IN RIQAS

Participation in RIQAS follows these simple steps:



Performance data is presented in a one page format with up to seven sub-reports.

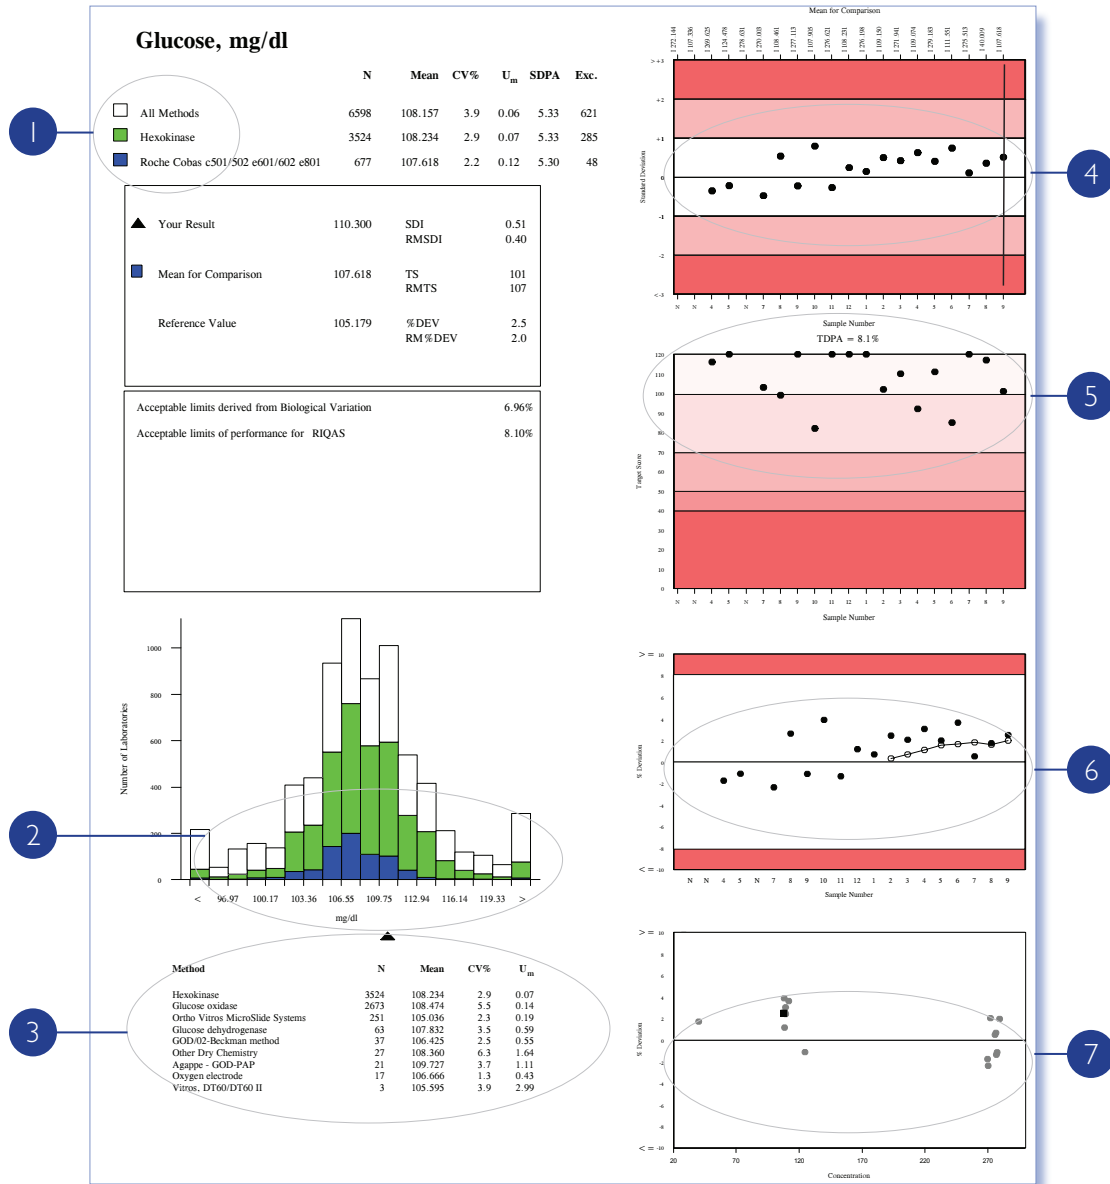

- 1 **Text Section:** Statistics for all methods, your method and instrument group (programme specific).
- 2 **Histogram:** Method and instrument comparison.
- 3 **Multi-Method Stat Section:** Enables assessment of the performance of each method.
- 4 **Levey-Jennings Chart:** Details features of your laboratory's performance.
- 5 **Target Score:** This unique chart provides a numerical index of performance, allowing at-a-glance assessment.
- 6 **%Deviation by Sample:** Helps to identify trends and shifts in performance.
- 7 **%Deviation by Concentration:** Rapid assessment of concentration related biases.

TEXT SECTION

The text section summarises the statistical information for each parameter.

Glucose, mg/dl		2	3	4	5	6	7
		N	Mean	CV%	U _m	SDPA	Exc.
<input type="checkbox"/>	All Methods	6598	108.157	3.9	0.06	5.33	621
<input checked="" type="checkbox"/>	Hexokinase	3524	108.234	2.9	0.07	5.33	285
<input checked="" type="checkbox"/>	Roche Cobas c501/502 e601/602 e801	677	107.618	2.2	0.12	5.30	48

▲	Your Result	110.300	SDI	0.51	9
			RMSDI	0.40	10
■	Mean for Comparison	107.618	TS	101	11
			RMTS	107	10
15	Reference Value	105.179	%DEV	2.5	12
			RM%DEV	2.0	10

Acceptable limits derived from Biological Variation		6.96%	13
Acceptable limits of performance for RIQAS		8.10%	14

Performance statement appears here if performance indicators exceed limits

RIQAS performance indicators include SDI, Target Score and %Deviation.

Acceptable performance criteria:

SDI < 2
 Target score ≥ 50
 %Deviation < defined acceptable limits

1 Report is presented in your chosen unit.

2 Number of returned results used to generate Mean for Comparison.

3 Average value of all laboratories' results.

4 Coefficient of Variation.

5 Uncertainty associated with the Mean for Comparison.

$$U_m = \frac{1.25 \times SD}{\sqrt{n}}$$

6 SDPA = Standard Deviation for Performance Assessment, calculated from the Target Deviation for Performance Assessment (TDPA) and the Mean for Comparison.

$$SDPA = \frac{TDPA \times \text{Mean for Comparison}}{t\text{-value} \times 100}$$

t-value = factor which represents the % of poor performers reflected in the TDPA (t-value ~ 1.645 when ~10% laboratories achieve poor performance), SDPA is combined with U_m, where appropriate.

If U_m > (0.3 × SDPA) then SDPA_{adjusted} = √(U_m² + SDPA²) and the reported value is suffixed with "a"

If U_m is less than (0.3 × SDPA) then SDPA_{adjusted} = SDPA

7 After statistical reduction, some results are excluded.

8 Ideally this will be your instrument group mean. If N<5 for instrument group, your method group Mean is selected as Mean for Comparison.

9 Standard Deviation Index = $\frac{\text{Your Result} - \text{Mean for Comparison}}{SDPA_{\text{adjusted}}}$

10 Running Mean average of the last 10 performance indicators is used to monitor performance over time and concentration range.

11 Target Score - The closer a value is to 120, the better the performance.

$$TS = \log_{10} \left(\frac{3.16 \times TDPA}{|\%Dev|} \right) \times 100$$

12 %Deviation from the Mean for Comparison -

$$\%Dev = \frac{\text{Your Result} - \text{Mean for Comparison}}{\text{Mean for Comparison}} \times 100$$

The closer the value is to zero, the better the performance.

13 Biological Variation stated for information purposes only.

14 Performance limit set for this parameter.

15 Reference values quoted for information purposes, where applicable.


HISTOGRAM

The Bar Graph is intended as a quick visualisation of how your lab's result compares to the method mean, instrument mean and all method mean.

All methods

Your method group


Your instrument group
(programme specific)

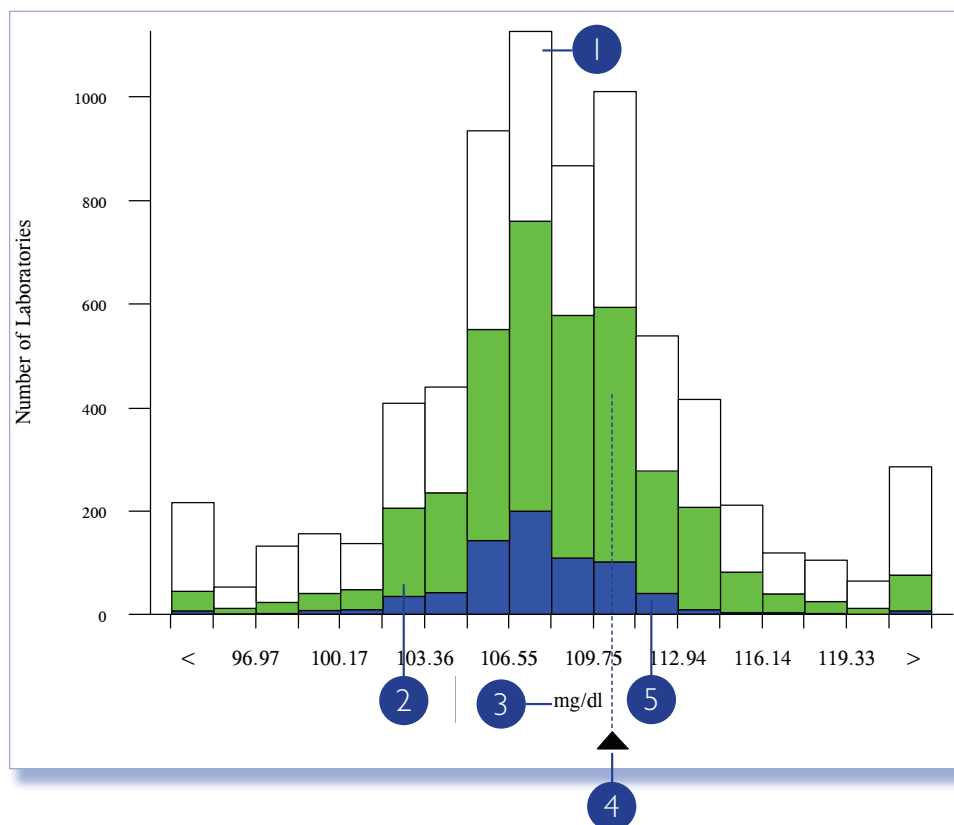

- 1 Total of 1126 laboratories reported values between 106.55 and 108.15.
- 2 200 laboratories reported values between 101.77 and 103.36 in your method group.
- 3 RIQAS reports show your unit of measurement.
- 4 Your result is indicated by the black triangle.
- 5 41 laboratories reported values between 111.35 and 112.94 in your instrument group.

LEVEY-JENNINGS CHART

SDIs reflect laboratory performance in relation to fit-for-purpose SDPAs and are useful to monitor performance over time. Acceptable performance is $SDI < 2$.

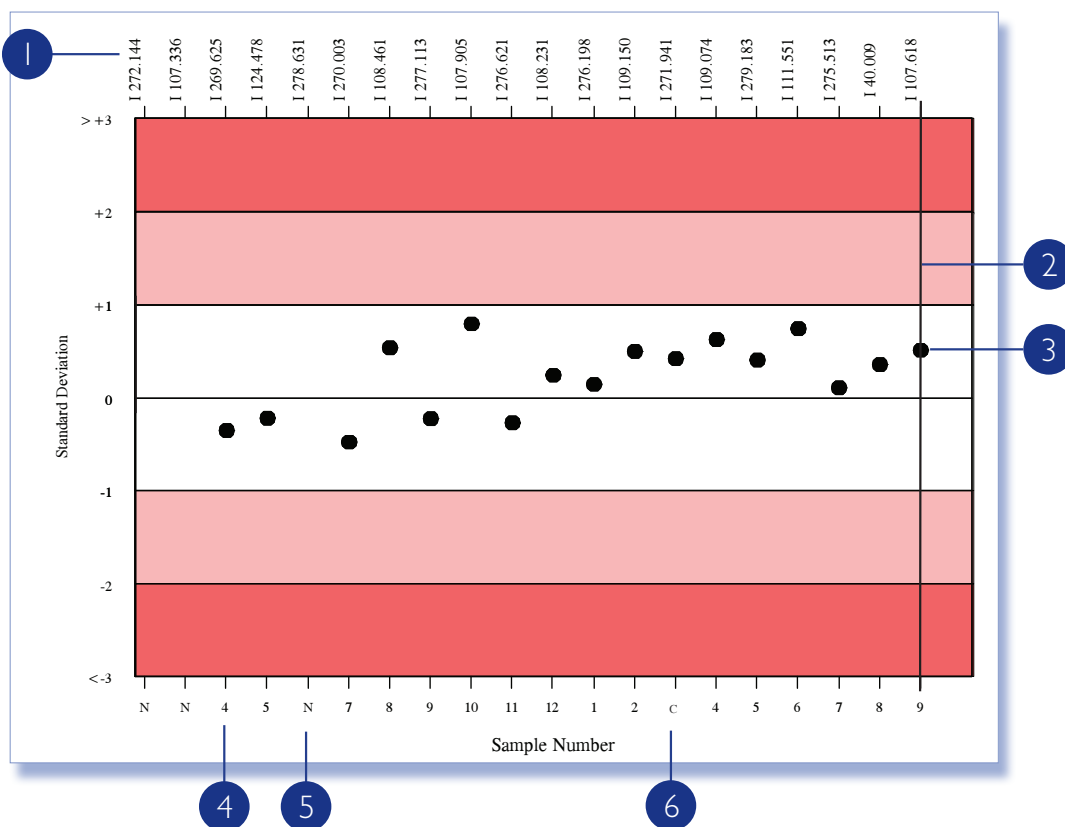


- 1 The Mean for Comparison for each sample is indicated at the top of the chart. This allows easy assessment of concentration related bias:
 - I: Instrument mean
 - M: Method mean
 - A: All method mean
- 2 This line indicates a change in registration details for this parameter.
- 3 Your SDI (Standard Deviation Index).

- 4 Sample number.
- 5 N = No result returned from your laboratory.
- 6 C = Corrected results will be accepted for non-analytical errors. Corrected results will be accepted up to 4 weeks after the final submission deadline, on application, with evidence of analysis. Late results are only accepted if there has been a Radox error.
 - R = Incorrect results can be removed retrospectively on request.

TARGET SCORE CHART

The Target Score (TS) allows you to assess your performance at a glance. The TS relates the %Deviation of your result from the Mean to a Target Deviation for Performance Assessment (TDPA). TDPA's are set to encourage participants to achieve and maintain acceptable performance. TDPA's are fit-for-purpose performance criteria which are set taking guidance from ISO/IEC 17043, ISO 13528 and IUPAC. Target Deviations for Performance Assessment are also used to calculate the Standard Deviation for Performance Assessment (SDPA).

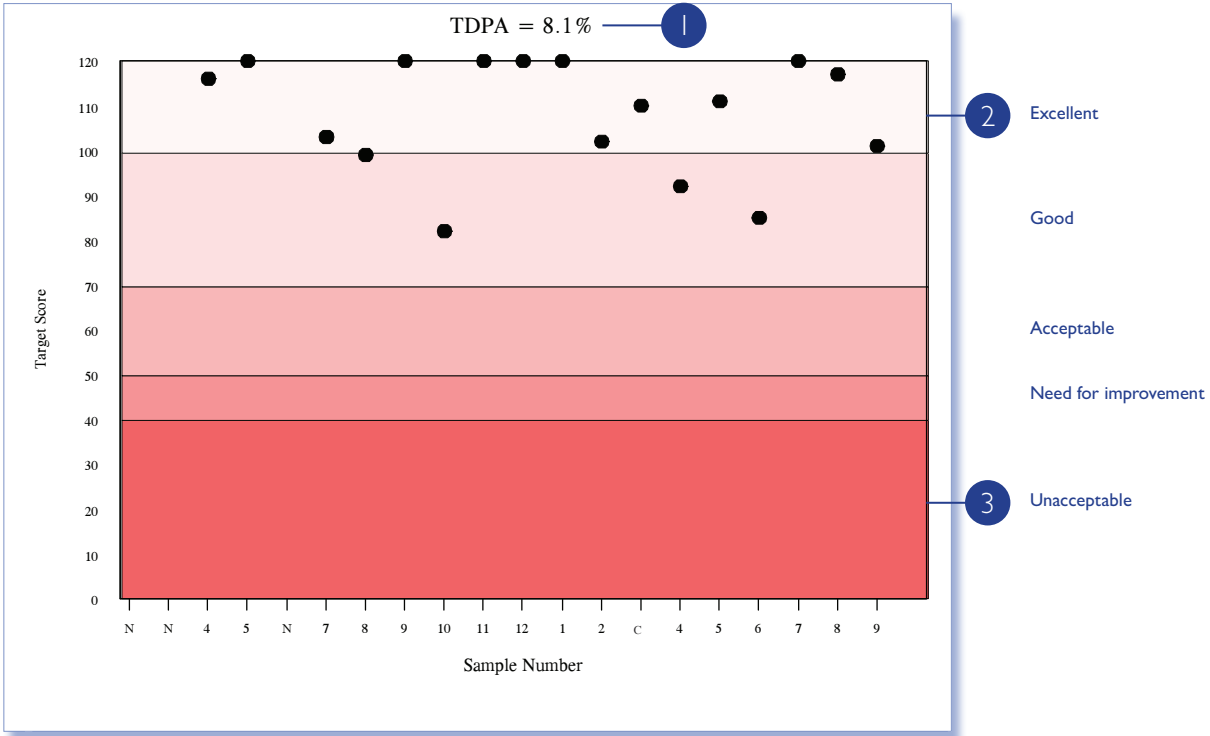

1 This is the upper deviation limit of performance for this parameter. TDPA's are reviewed regularly and deemed fit for purpose by the RIQAS Advisory Panel.


2 High scores ≥ 50 in the lighter shaded area represent acceptable, good or excellent performance.

3 Heavy shading for values 10 to 50 signifies poor performance.

%DEVIATION CHARTS


The %Deviation by sample chart helps to identify trends and shifts in performance.

$$\%Deviation = \frac{\text{Your Result} - \text{Consensus Mean}}{\text{Consensus Mean}} \times 100\%$$

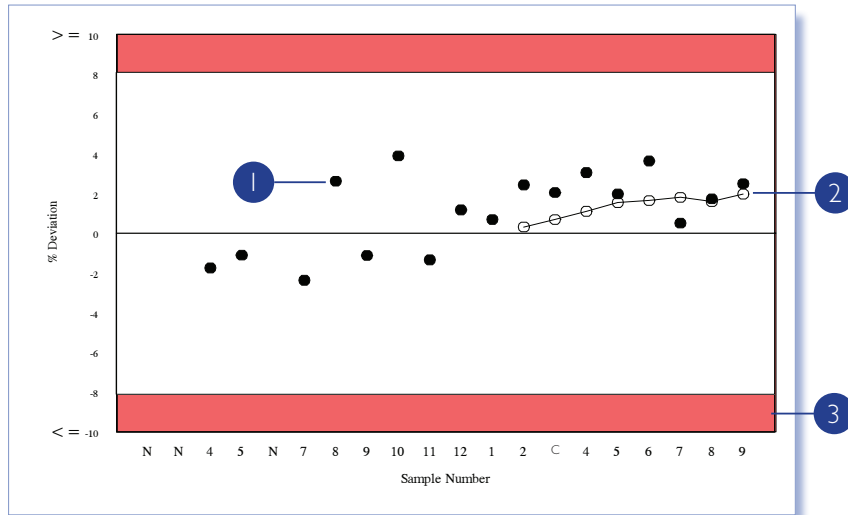

- 1 %Deviation from Mean for Comparison.
- 2 Plot of Running Mean %Deviations (average of the last 10 %Deviations for the sample indicated).
- 3 Acceptable limits of performance. These are defaulted to RIQAS TDPAs but can be set to e.g. biological variation or regulatory requirement on request.

The %Deviation by concentration chart enables rapid assessment of concentration related biases. Biases at low or high concentrations can be easily determined.

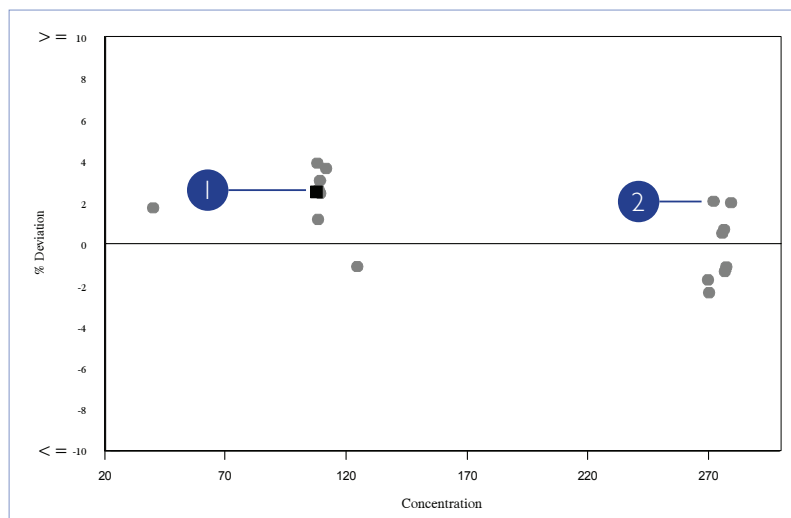

- 1 Current sample indicated by square.
- 2 %Deviation at specific concentration.

MULTI-METHOD STAT SECTION

This section provides an easy way of assessing the performance of other methods used to analyse the parameter in question.

Method	N	Mean	CV%	U_m
Hexokinase	3524	108.234	2.9	0.07
Glucose oxidase	2673	108.474	5.5	0.14
Ortho Vitros MicroSlide Systems	251	105.036	2.3	0.19
Glucose dehydrogenase	63	107.832	3.5	0.59
GOD/02-Beckman method	37	106.425	2.5	0.55
Other Dry Chemistry	27	108.360	6.3	1.64
Agappe - GOD-PAP	21	109.727	3.7	1.11
Oxygen electrode	17	106.666	1.3	0.43
Vitros, DT60/DT60 II	3	105.595	3.9	2.99

SUMMARY PAGE

Located at the back of the RIQAS Report, the Summary Page collates the key information, allowing participants to review the performance of all parameters at-a-glance.

Analyte	Mean for Comparison	Your Result	SDI	RMSDI	%DEV	RM%DEV	TS	RMTS	Performance
Albumin	2.120	2.230	1.00	0.37	5.2	2.0	72	107	
Alkaline Phosphatase	17.705	19.000	0.61	-0.27	7.3	-2.9	93	105	
ALT (GPT)	12.387	12.000	-0.33	-0.47	-3.1	-3.8	119	103	
Amylase, Total	20.454	22.000	0.72	-0.29	7.6	-2.5	86	103	
AST (GOT)	11.976	11.000	-0.86	-0.03	-8.2	-0.4	78	100	
Bicarbonate	8.203	6.900	-1.48	0.15	-15.9	1.5	54	98	
Bilirubin, Direct	0.251	0.380	<u>2.57</u>	2.64	<u>51.3</u>	47.2	<u>31</u>	29	▲
Bilirubin, Total	0.701	0.640	-0.91	-0.29	-8.8	-2.9	76	101	
Calcium	6.074	6.020	-0.19	-0.40	-0.9	-1.8	120	92	
Chloride	76.353	77.000	0.30	-0.28	0.8	-0.8	120	98	
Cholesterol	112.696	110.000	-0.55	0.05	<u>2.4</u>	0.2	97	115	
CK, Total	111.659	111.000	-0.08	0.35	-0.6	2.5	120	107	
Creatinine	0.607	0.620	0.27	0.06	2.1	0.5	120	117	
Glucose	36.429	36.000	-0.26	-0.84	-1.2	-3.7	120	82	
HDL-Cholesterol	98.836	102.000	0.21	-0.04	3.2	-0.4	120	113	
Iron	97.374	99.000	0.28	0.01	1.7	0.1	120	114	
Lactate		No Result		Too Few		Too Few	N/A	N/A	
LD (LDH)	85.894	87.000	0.11	-0.70	1.3	-6.3	120	89	
Magnesium	1.313	1.390	0.79	-0.07	5.8	-0.5	82	107	
Phosphate, Inorganic	1.451	1.540	1.02	0.02	6.1	0.1	71	112	
Potassium	1.770	1.840	1.10	-0.25	3.9	-0.7	67	99	
Protein, Total	3.850	3.830	-0.11	0.07	-0.5	0.3	120	114	
Sodium	112.537	114.000	0.58	-0.01	1.3	-0.0	95	104	
TIBC	133.143	133.000	-0.01	-0.01	-0.1	-0.1	120	117	
Trig Total	23.626	24.000	0.18	-0.09	1.6	-0.6	120	114	
Urea	5.872	5.000	<u>-2.02</u>	-0.57	<u>-14.9</u>	-4.0	<u>41</u>	95	▲
Uric Acid (Urate)	3.135	3.100	-0.20	-0.44	-1.1	-2.4	120	107	

ORMSDI -0.05

ORM%DEV 0.8

ORMTS 102

1 RMSDI - is the Running Mean of the 10 previous SDIs (if fewer than 10 results on file, "Too Few" is printed).

2 RM %DEV - Average of the last 10 %DEV for this parameter.

3 RMTS - Average of the last 10 Target Scores for this parameter.

4 Red triangle appears when all performance indicators (SDI, %DEV and TS) exceed acceptable performance, i.e: when
SDI > 2
TS < 50
%DEV > acceptable limits set


5 Overall RMSDI = average RMSDI for this sample distribution.

6 Overall RM%DEV = average RM%DEV for this sample distribution.

7 Overall RMTS = average RMTS for this sample distribution.

MULTI-INSTRUMENT REPORT

Register up to five instruments per programme at no extra cost. In addition to a standard report for each instrument, a multi-instrument report is also provided allowing comparative performance assessment.

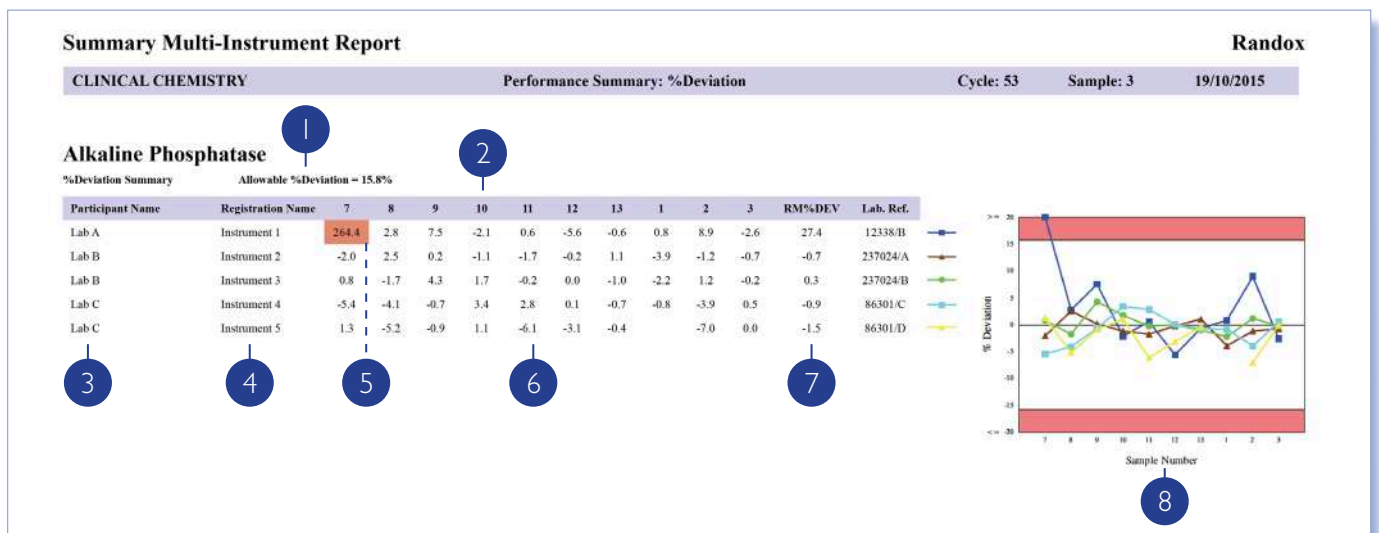

- 1 Allowable %deviation for the parameter in question, based on the RIQAS TDPA.
- 2 Sample number.
- 3 Lab name.
- 4 Unique instrument ID.

- 5 Poor performance.
- 6 %Deviation for each individual sample.
- 7 RM %Dev - Average of the last 10 %Dev for this parameter.
- 8 %Deviation chart comparing the performance of each instrument.

URINE TOXICOLOGY REPORT

Laboratory performance is presented in both quantitative and qualitative screening formats, allowing for easy interpretation at-a-glance.


Screening Section

Quantitative Section

Amphetamines Group, ng/ml

Your Result Negative

Based on weighed-in value of 375
and your chosen cut-off value of 500
the correct response was Negative

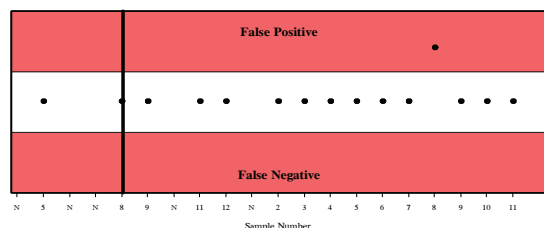


□ All Methods
■ KIMS

N	Mean	CV%	U _m	SDPA	Exc.
45	386.683	19.1	13.78	73.94	4
17	357.294	18.6	20.14	69.41a	1

▲ Your Result	352.000	SDI	-0.08
		RMSDI	Too Few
■ Mean for Comparison	357.294		

d-Amphetamine	375	ng/ml
Ethanol	45	mg/dl
LSD	1.25	ng/ml
EDDP	225	ng/ml
Buprenorphine	7.5	ng/ml

	Cut-off	TN	TP	FN	FP	RC	NT	Total
Your Result	500	1	0	0	0	0	0	1
KIMS	300	0	1	0	0	0	0	1
	500	12	0	0	0	0	0	12
	1000	9	0	0	0	0	0	9
	All	21	1	0	0	0	0	22
All Methods	150	0	1	0	0	0	0	1
	300	0	7	0	0	0	0	7
	500	31	0	0	3	0	0	34
	1000	62	0	0	6	0	0	68
	All	93	8	0	9	0	0	110
Competitive Antibody Binding	500	0	0	0	1	0	0	1
CEDIA	500	4	0	0	0	0	0	4
Chemiluminescence	500	1	0	0	0	0	0	1
DRI-EIA	500	4	0	0	1	0	0	5
EMIT	500	8	0	0	0	0	0	8
FPIA	500	1	0	0	0	0	0	1
Point of Care	500	1	0	0	0	0	0	1
Randox Biochip Array Technology	500	0	0	0	1	0	0	1

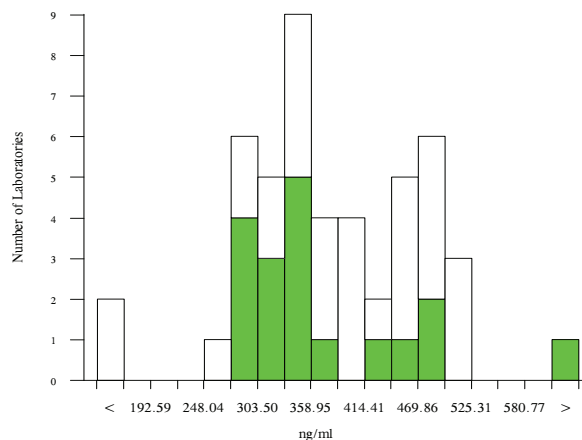



Method	N	Mean	CV%	U _m
KIMS	17	357.294	18.6	20.14
EMIT	9	344.440	12.4	17.74
Competitive Antibody Binding	7	460.857	8.9	19.30
DRI-EIA	7	433.767	17.2	35.31
CEDIA	2	410.000	11.7	42.25

Performance History

Your Data (Last 10 Samples)	Your Method (This Sample)	Your Method (Last 10 Samples)	All Methods (This Sample)	All Methods (Last 10 Samples)
0 % False Negatives	0 % False Negatives	1 % False Negatives	0 % False Negatives	8 % False Negatives
10 % False Positives	0 % False Positives	11 % False Positives	8 % False Positives	7 % False Positives
90 % Correct Responses	100 % Correct Responses	88 % Correct Responses	92 % Correct Responses	85 % Correct Responses

URINE TOXICOLOGY REPORT SCREENING SECTION


Qualitative comparison of screening results available for each parameter.

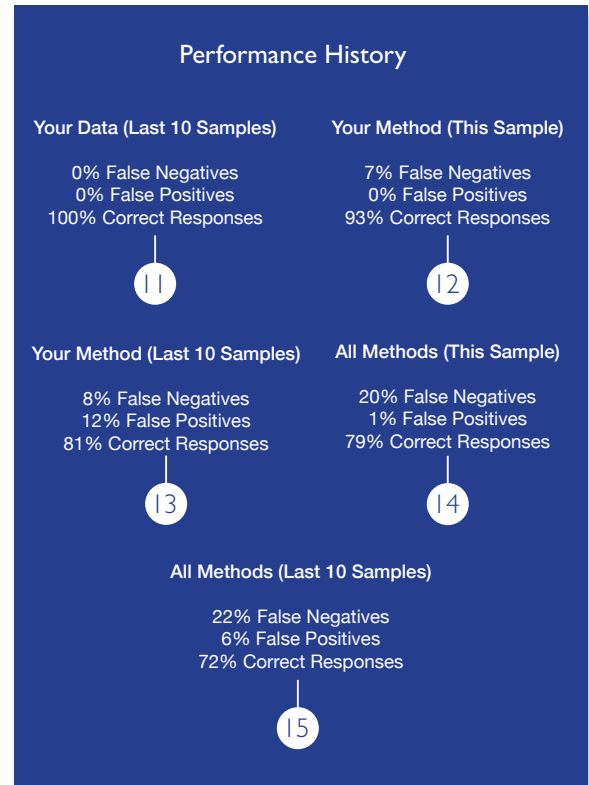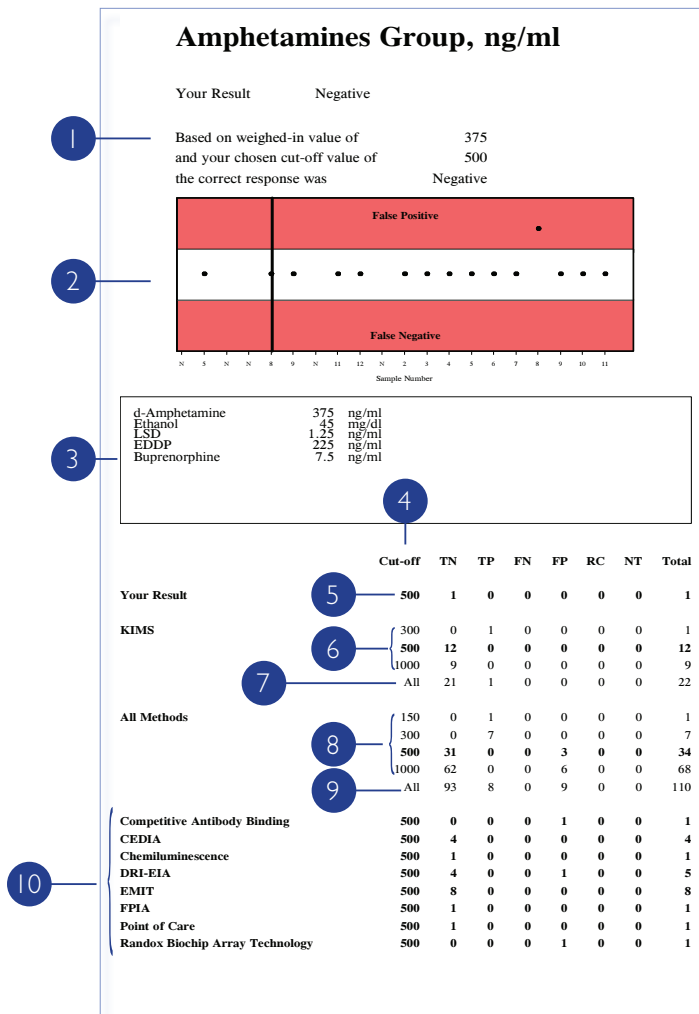

- Text section shows the correct response for the lab based on a comparison between the weighed in value and the lab's cut off value.
- Screening Results:** This chart is a quick visualisation of your performance over the last 20 samples. A result in the white section indicates a correct response. A result in the upper red section indicates a False Positive response, and a result in the lower red section indicates a False Negative response.
- Comment section for RIQAS to provide your laboratory with additional relevant information regarding this sample, such as spiked metabolite concentration.
- Screening result response categories. All abbreviations indicated at the bottom of the report page.
Key
TN - true negative TP - true positive FN - false negative
FP - false positive RC - sent for confirmation NT - not tested
- Screening Summary:** Your screening result shown in the appropriate response category and your cut off for this sample.
- Screening results for all cut-offs returned for this sample within your method group.
- Total screening results over all your cut-offs for your laboratory's method.
- Screening results for all cut-offs returned for this sample over all methods.
- Total screening results over all cut-offs for all methods.
- Screening results for other methods using same cut-off as your laboratory.
- Performance history for this parameter; based on previous 10 samples.
- Performance of your method over all cut-offs for this sample.
- Performance history of your method over all cut-offs, based on the previous 10 samples.
- Performance of all methods over all cut-offs for this sample.
- Performance history of all methods over all cut-offs, based on the previous 10 samples.

URINE TOXICOLOGY REPORT QUANTITATIVE SECTION

Quantitative statistical comparison available for each parameter.

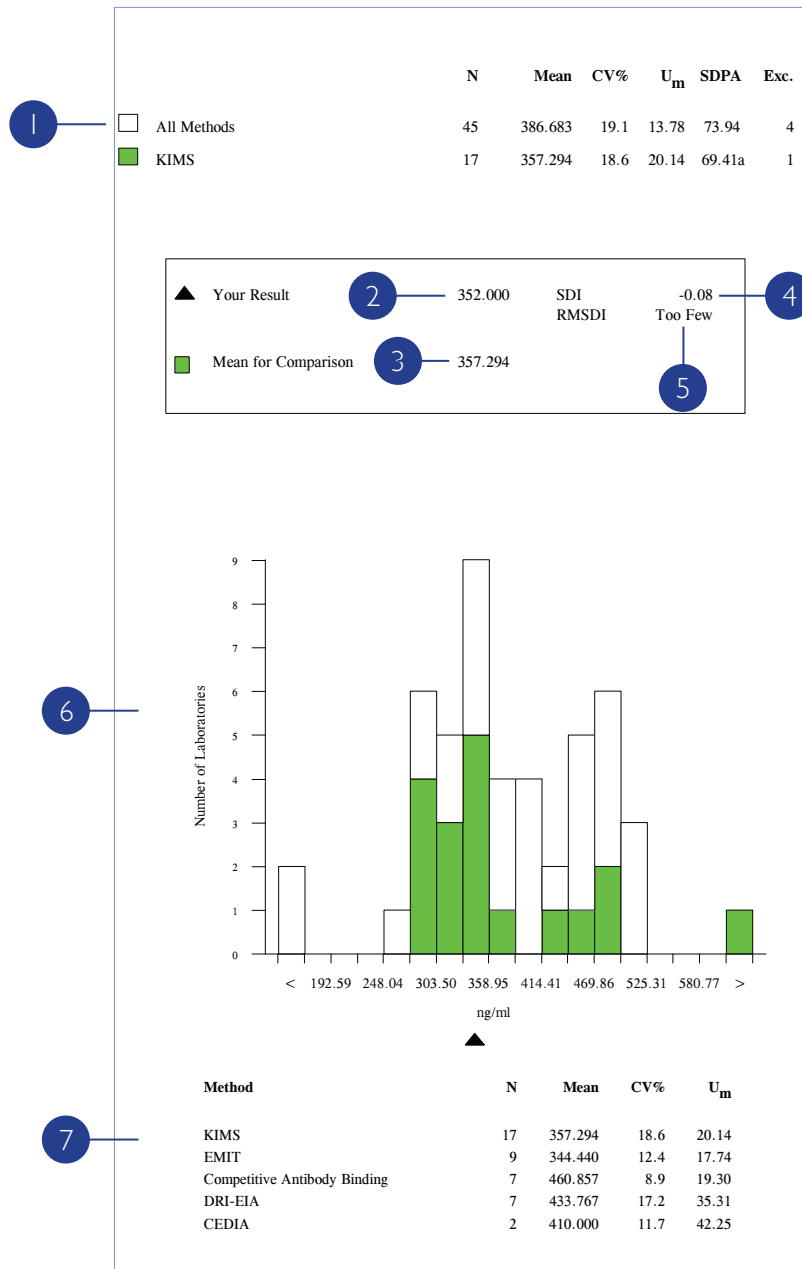

1 **Quantitative Text Section:** Comparison statistics. Caution is needed when the N value is too small to support statistical significance.

2 Your Result.

3 Your Mean for Comparison.

4 **Standard Deviation Index** = $\frac{(\text{Your Result} - \text{Mean for Comparison})}{\text{SD of Mean for comparison}}$

5 Running mean SDI = average of last 10 SDIs for this parameter (If fewer than 10 results, "Too Few" is printed).

6 **Quantitative Results Histogram:** This graph provides a quick visualisation of how your quantitative result falls into the overall picture for all methods and your method group.

7 All available method statistics for this sample.

Your performance for each parameter is presented in a simple, convenient report.

Screening Results



- 1 Categories are stated in your unit.
- 2 Your method group.
- 3 Your categories (available result options for chosen test strip and unit).
- 4 All categories (result options) available for this parameter for any method (test strip).
- 5 Results from all methods (test strips) returning results in the same categories as your lab.
- 6 Results from all methods for all available categories.
- 7 Your Result.
- 8 **Your Score:** Scores between 0-6 are acceptable, 7 borderline and 8 - 10 unacceptable.
- 9 Target category and percentage of submitted results in that category.
- 10 Performance Statement.
- 11 **Comments Box:** Provides number of correct scores and acceptable assessments for the last 6 samples.
- 12 **Categories Histogram:** A quick visualisation of how your lab's result falls into the overall picture for your categories.
- 13 Possible reporting categories for your method.
- 14 Your result is indicated by the black triangle.
- 15 **Levey-Jennings Chart:** Acceptable scores (0-6) have no shading, borderline scores (7) have light red shading, unacceptable scores (8-10) have dark red shading.
- 16 Score for each sample number.
- 17 Sample Number.
- 18 Target Categories.
- 19 All methods reported for this parameter.
- 20 **Detailed summary of results:** This table enables you to see how you compare to all other results.

SEROLOGY: SCREENING (QUALITATIVE) REPORT

Your performance for multiple samples is presented in a convenient single report per quarterly distribution.

Anti-HIV-1&2 Combi


Sample 1

Your method: Roche Cobas 6000 / 8000
 Your result: Reactive
 Acceptable result (Method): Reactive

Overall results

Non-Reactive: 91
 Inconclusive: 24
 Reactive: 542

Method	N	Non-Reactive	Inconclusive	Reactive
Abbott Architect	212	4	13	195
Roche Cobas 6000 / 8000	129	4	0	125
Roche Cobas 4000/e411	118	2	3	113
Siemens Centaur XP/XPT/Classic	44	18	3	23
BioMerieux VIDAS	27	1	2	24
Ortho Vitros 3600/5600/ECi	22	20	0	2
Beckman Dxi 600 / 800	17	0	0	17
Diasorin/Abbott Murex ELISA	10	9	1	0
Diasorin Liaison	10	0	0	10
Bio-Rad HIV assays	8	6	0	2
Alere Determine HIV-1/2	7	4	0	3
Siemens Enzygnost	7	2	0	5
Beckman Access/LXi725	6	0	1	5
Roche Elecsys	5	0	0	5
SD Bioline Rapid Test HIV	5	3	0	2
Roche Modular E170	4	0	0	4
Beckman Access/Biorad HIV Combo	3	0	1	2
Diagnostic BioProbes ELISA	3	0	0	3
Vector Based ELISA	3	2	0	1
Siemens Centaur CP	2	1	0	1
Diagnostic Automation Inc HIV1/2	2	2	0	0
J Mitra/Diagnostic Enterprises TRI-DOT	2	2	0	0
Fujirebio Serodia Particle Agg.	2	2	0	0

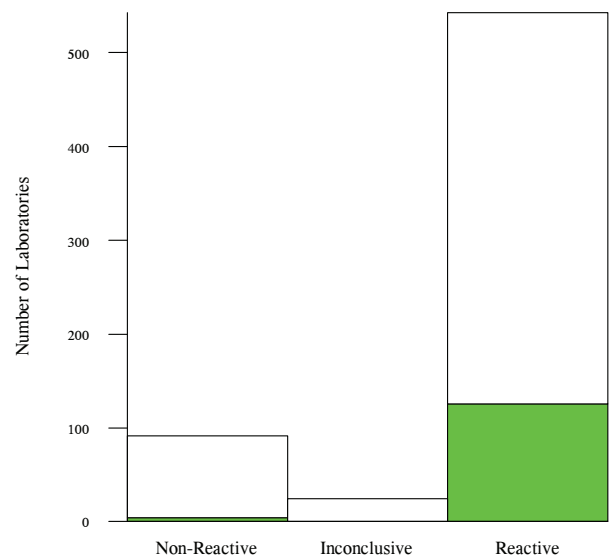

1 Your qualitative result and chosen method are presented along with the acceptable result based on an 80% consensus. This consensus will be at the method level if there are >5 labs in the group or if there are <5 labs, will be at the all method level.

2 Overall Summary shows the number of results for this parameter and sample which are non-reactive, inconclusive or reactive.

3 Your Result is shown as a black triangle on the category chart compared to other laboratories in groups:

All Methods Your Method

4 Summary shows performance of all the methods used to analyse the parameter.

SEROLOGY: SCREENING (QUANTITATIVE) REPORT


Your performance for multiple samples is presented in a convenient single report per quarterly distribution.

Anti-Rubella IgG, IU/ml

Sample 2

	N	Mean	CV%	U _m	SDPA	Exc.
All methods	210	92.574	37.2	2.97	34.42	31
Abbott Architect	39	83.219	8.7	1.46	7.27	5


▲ Your Result	84.800	SDI RMSDI	0.22 Too Few
■ Mean for Comparison	83.219		

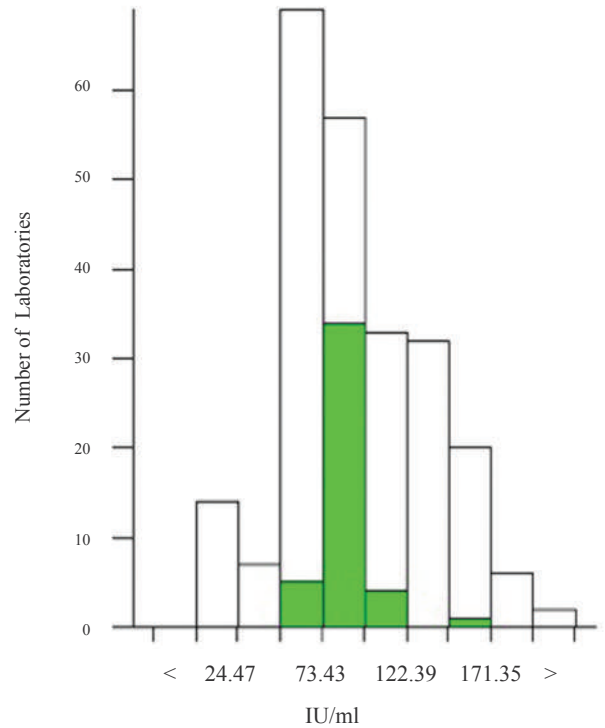

3

Method	N	Mean	CV%	U _m
Biomerieux VIDAS	48	150.979	9.8	2.97
Abbott Architect	44	83.219	8.7	1.46
Roche Cobas 6000/8000	18	58.792	3.6	0.68
Abbott AxSYM	17	108.206	18.0	6.09
Siemens/DPC Immulite 2000/2500	17	90.800	6.2	1.94
Roche Cobas 4000/e411	17	59.973	7.0	1.35
Siemens/Bayer ADVIA Centaur	14	120.775	11.0	5.88
Roche Elecsys	11	57.043	3.9	1.05
Diasorin Liaison	9	52.388	18.0	4.16
Roche Modular E170	9	58.949	3.9	1.08
Beckman DxI 600/800	6	125.817	7.4	4.75

4

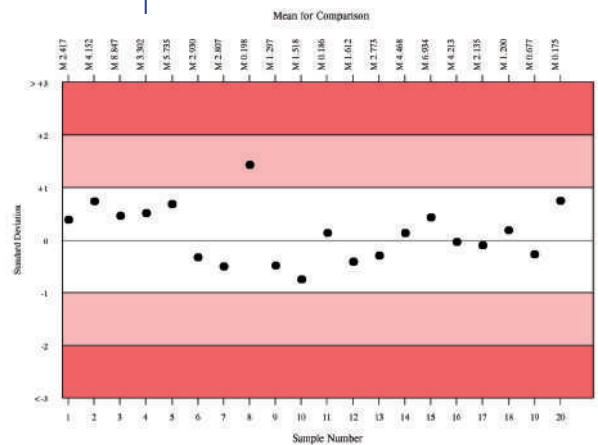

1 Quantitative statistics for All Methods and Your Method are presented in your chosen unit along with your result and your performance scores (SDI and RMSDI).

2 Your result is presented on the bar graph as a black triangle, showing how you compare to:

All Methods Your Method

3 Multi Method Statistics section provides an easy way of assessing the performance of the methods used to analyse the parameter.

4 **Levey-Jennings chart** - Your SDIs for previous 20 samples.

QUANTITATIVE (END-OF-CYCLE REPORT)

The End-of-Cycle Report is sent to labs receiving standard reports at the end of each cycle and provides a complete summary of statistics. Results can also be compared to the previous cycle.

Albumin, g/l

Method: Bromocresol Purple
Instrument: Siemens/Dade Dimension RxL/Max/Xpand
Reagent: Siemens/Dade Behring

RIQAS TDPa: 7.1% **Biological Variation:** 3.9%

Sample	Result	Unit	N	Mean for Comparison	CV%	Um	SDPA	SDI	TS	%Deviation
1	28.200	g/l	68	I 28.013	2.4	0.10	1.26	0.15	120	0.67
2	26.900	g/l	87	I 26.853	2.7	0.10	1.21	0.04	120	0.17
3	39.900	g/l	71	I 40.531	2.5	0.15	1.82	-0.35	118	-1.56
4	19.200	g/l	81	I 19.429	2.5	0.07	0.87	-0.26	120	-1.18
5	41.700	g/l	67	I 41.859	2.0	0.13	1.88	-0.08	120	-0.38
6	57.300	g/l	87	I 57.257	2.7	0.21	2.58	0.02	120	0.08
7	45.000	g/l	72	I 45.850	2.1	0.14	2.06	-0.41	110	-1.85
8	27.600	g/l	87	I 28.013	2.5	0.09	1.26	-0.33	120	-1.47
9	41.200	g/l	70	I 41.891	2.2	0.14	1.88	-0.37	115	-1.65
10	26.900	g/l	83	I 26.742	3.3	0.12	1.20	0.13	120	0.59
11	40.700	g/l	71	I 40.601	2.2	0.14	1.83	0.05	120	0.24
12	45.100	g/l	80	I 45.456	2.2	0.14	2.04	-0.17	120	-0.78
13	27.300	g/l	63	I 28.179	2.0	0.09	1.27	-0.69	87	-3.12

Cycle 45 Cycle 46

Cycle Average SDI -0.23 -0.18
Cycle Average TS 110 116
Cycle Average %DEV -1.05 -0.79

Cycle Average Absolute SDI 0.36 0.24
Cycle Average Absolute %DEV 1.63 1.06





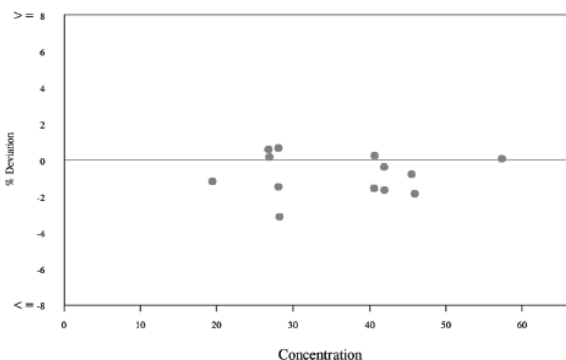


CHART SECTION (END-OF-CYCLE REPORT)

Your results for current cycle shown in various diagrams.

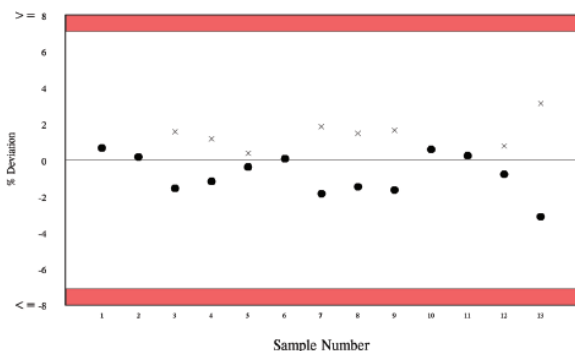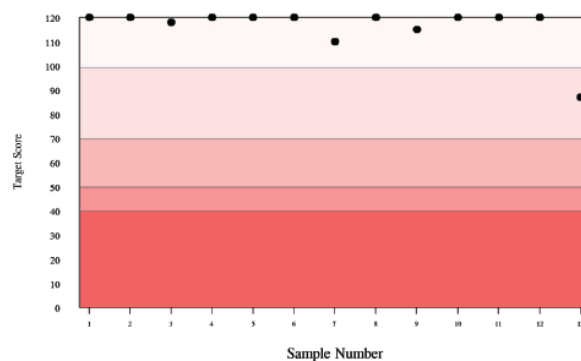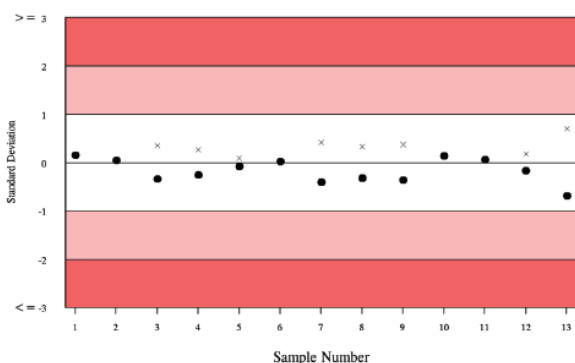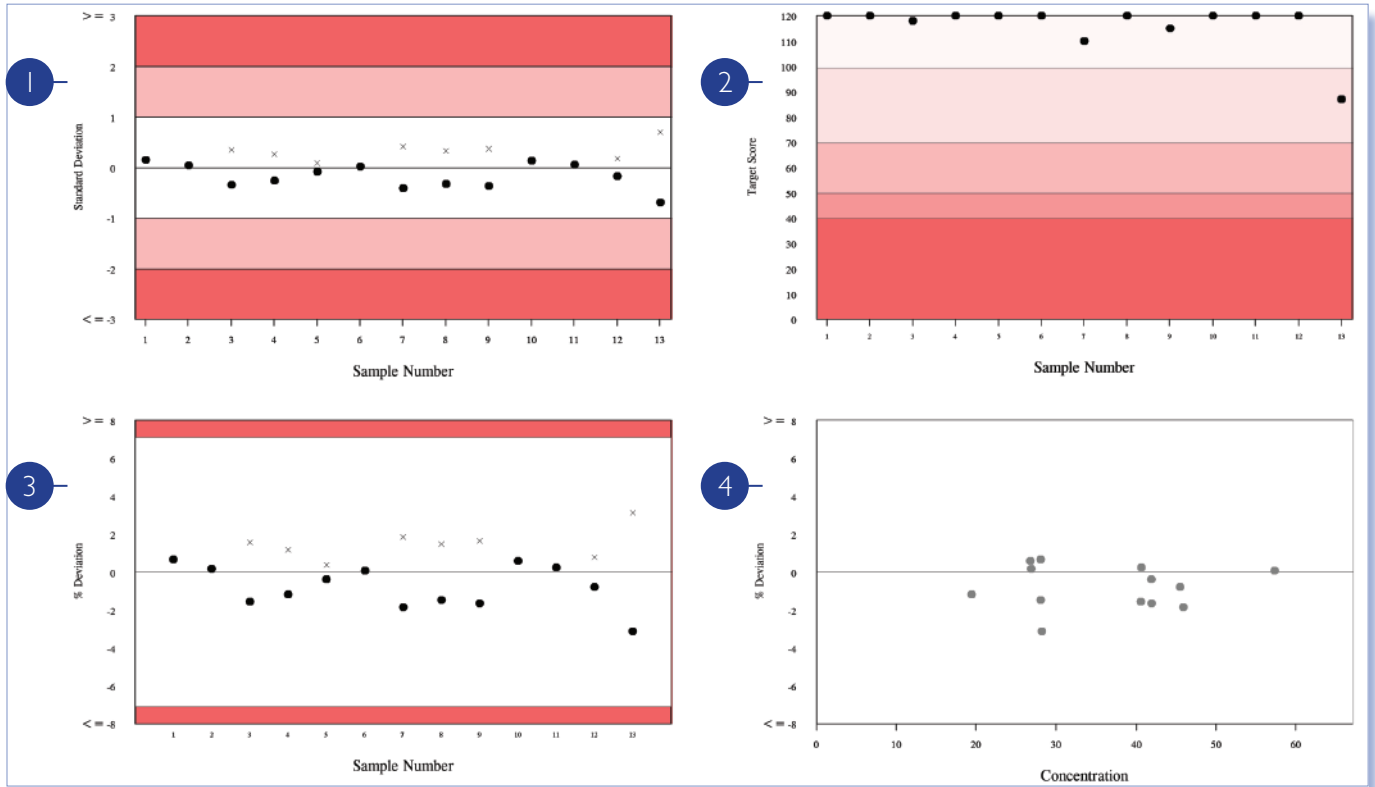

- | | | |
|---|-----------------------------------|--|
| 1 | Levey-Jennings chart | Shows your SDIs for a full cycle. <ul style="list-style-type: none"> • Shows SDI (positive and negative) x Shows absolute SDI |
| 2 | Target Score chart | Shows your Target Scores for a full cycle. |
| 3 | %Deviation by sample chart | Shows your %Deviations for a full cycle. <p>Acceptable limits equal to TDPA unless alternative limits are registered by the lab.</p> <ul style="list-style-type: none"> • Shows %Deviation (positive and negative) x Shows absolute %Deviation |
| 4 | %Deviation by Concentration chart | Shows your results for a full cycle. |

TEXT SECTION (END-OF-CYCLE REPORT)

The text section summarises the statistical information for all samples.

1 Albumin, g/l

Method: Bromocresol Purple
Instrument: Siemens/Dade Dimension RxL/Max/Xpand
Reagent: Siemens/Dade Behring

3 RIQAS TDPA: 7.1% **Biological Variation:** 3.9%



Your assay details at the end of the cycle. The RIQAS TDPA and biological variation for the parameter are shown if available.

- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13
- 14

Sample	Result	Unit	N	Mean	SDPA	U _m	CV%	SDI	TS	% Deviation
1	28.200	g/l	68	I 28.013	1.26	0.10	2.4	0.15	120	0.7
2	26.900	g/l	87	I 26.853	1.21	0.10	2.7	0.04	120	0.2
3	39.900	g/l	71	M 40.531	1.82	0.15	2.5	-0.36	116	-1.5
4	19.200	g/l	81	I 19.429	0.87	0.07	2.5	-0.27	120	-1.2
5	41.700	g/l	67	I 41.942	1.88	0.13	2.0	-0.09	120	-0.4
6	57.300	g/l	87	I 57.257	2.58	0.21	2.7	0.02	120	0.1
7	45.000	g/l	72	I 45.850	2.06	0.14	2.1	-0.43	108	-1.8
8	27.600	g/l	87	I 28.011	1.26	0.09	2.5	-0.34	118	-1.5
9	41.200	g/l	70	I 41.823	1.88	0.14	2.2	-0.38	113	-1.6
10	26.900	g/l	83	I 26.742	1.20	0.12	3.3	0.14	120	0.6
11	40.700	g/l	71	I 40.601	1.83	0.13	2.2	0.06	120	0.2
12	45.100	g/l	80	I 45.119	2.05	0.14	2.2	-0.18	120	-0.8
13	27.300	g/l	63	I 28.454	1.27	0.09	2.0	-0.72	86	-3.1



Summary of your results and statistics are shown, including Mean for Comparison, SDPA, %CV, U_m, SDI, Target Score, %Deviation.

	Cycle 45	Cycle 46
15 Cycle Average SDI	-0.23	-0.18
Cycle Average TS	110	116
Cycle Average %DEV	-1.05	-0.79
16 Cycle Average Absolute SDI	0.36	0.24
Cycle Average Absolute %DEV	1.63	1.06



Table containing a summary of your performance for previous cycle and current cycle, including Average Absolute SDIs and %Deviations.

TEXT SECTION (END-OF-CYCLE REPORT)

- 1 Report presented in your chosen unit
- 2 Your assay details as of the last sample
- 3 RIQAS TDPA and Biological variation
- 4 Sample number
- 5 Your results for each sample
- 6 Unit your result was returned in
- 7 Number of results used for statistical analysis
- 8 Mean for Comparison
- 9 SDPA = Standard Deviation for performance assessment
- 10 Uncertainty of Mean for Comparison
- 11 Coefficient of Variation (%)
- 12 Your Standard Deviation Index
- 13 Your Target Score
- 14 Your %Deviation

- 15 Cycle average of your performance indicators – Standard Deviation Index, Target Score and %Deviation.

$$\text{Cycle Average SDI} = \frac{\text{(Sum of SDIs returned for the completed cycle)}}{\text{(Number of samples returned in cycle)}}$$

$$\text{Cycle Average Target Score} = \frac{\text{(Sum of your Target Scores returned for the completed cycle)}}{\text{(Number of samples returned in cycle)}}$$

$$\text{Cycle Average \%Deviation} = \frac{\text{(Sum of your \%Deviations returned for the completed cycle)}}{\text{(Number of samples returned in cycle)}}$$


- 16 Cycle average for Absolute values of your SDI and %Deviation. Absolute values show how far a value is from zero regardless of the sign. This is an indication of the magnitude of accuracy.

$$\text{Cycle Average Absolute SDI} = \frac{\text{(Sum of your Absolute SDIs returned for the completed cycle)}}{\text{(Number of samples returned in cycle)}}$$

$$\text{Cycle Average Absolute \%Deviation} = \frac{\text{(Sum of your Absolute \%Deviations returned for the completed cycle)}}{\text{(Number of samples returned in cycle)}}$$

CURRENT & PREVIOUS CYCLE ABSOLUTE SDIs (END-OF-CYCLE REPORT)

Based on the cycle average absolute SDI, this chart provides a visual representation of your laboratory's performance compared to the previous cycle.

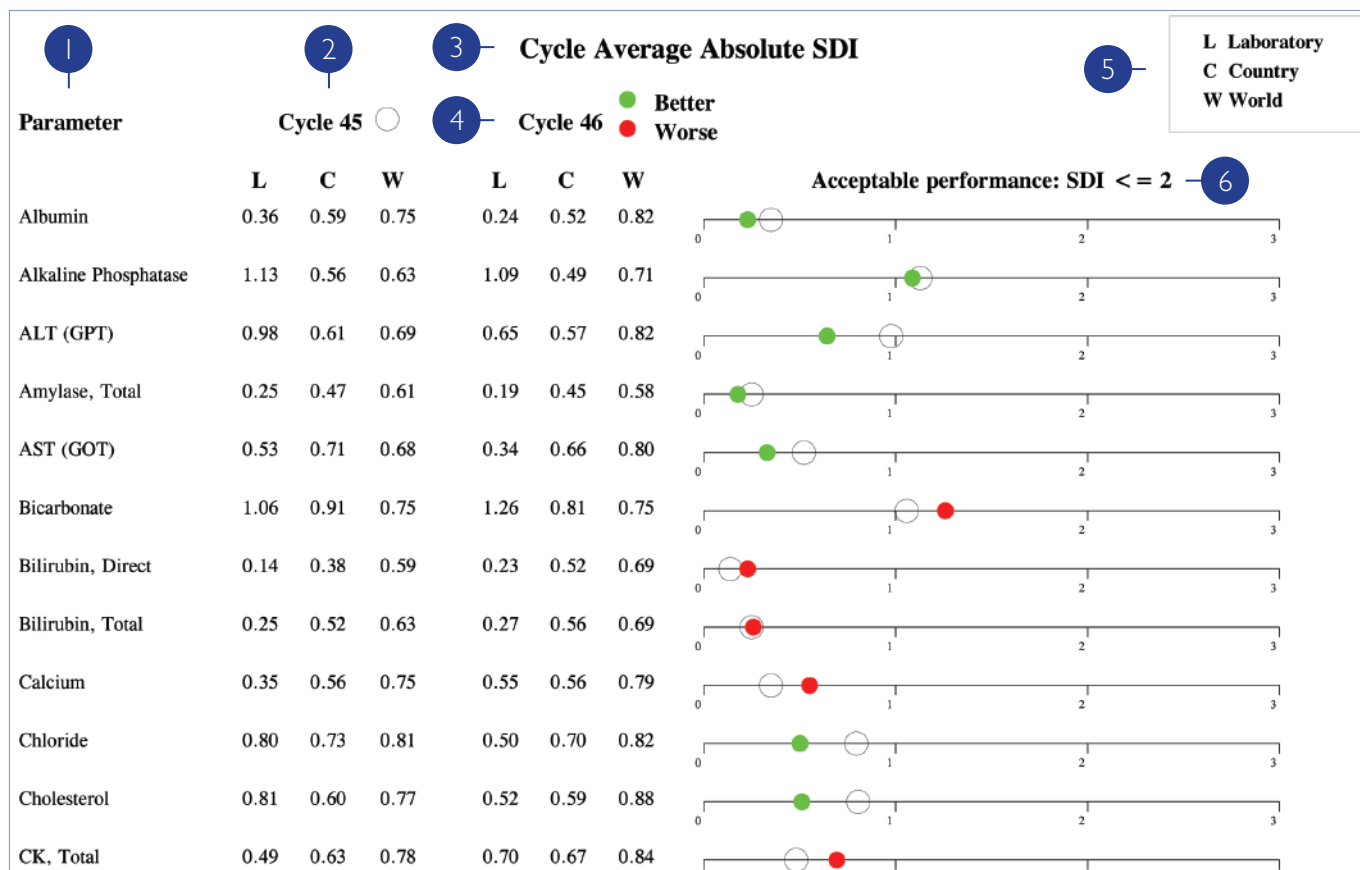

- 1 Parameter list
List of all parameters registered.
- 2 Results for previous cycle
Indicated by open circle on the chart.
- 3 Report title - Cycle Average Absolute SDI
This shows your performance this cycle compared to the previous cycle.
- 4 Results for current cycle
Indicated by a closed circle on the chart.
- 5 Legend
Cycle Average Absolute SDIs are shown for:
 - L Your results throughout the cycle
 - C All labs within your own country
 - W All labs Worldwide

- 6 Graphical representation of Absolute SDIs
Acceptable performance is ≤ 2.
If Absolute SDI for current cycle is less than that for the previous cycle, this is indicated by a green circle.
If Absolute SDI for current cycle is greater than that for the previous cycle, this is indicated by a red circle.
The closer the circle is to zero, the better the performance.

CERTIFICATE OF PERFORMANCE (END-OF-CYCLE REPORT)

An End-of-Cycle report will be issued for all registrations. However, the Certificate of Performance will only be available for parameters where results for at least 50% of samples in the cycle have been returned. Labs joining after the beginning of the cycle will only receive the Certificate of Performance if they meet this criterion. Any parameters not included on the Certificate of Acceptable Performance will be listed on the Notification of Unacceptable Performance.



RANDOX INTERNATIONAL QUALITY ASSESSMENT SCHEME

CERTIFICATE OF ACCEPTABLE PERFORMANCE

RIQAS Department
Randox Laboratories
CRUMLIN
COUNTY ANTRIM
BT29 4QY
UNITED KINGDOM

1

2 LABORATORY REF. NO. XX/X

3 CLINICAL CHEMISTRY - CYCLE 47

4 11/03/2013

This is to certify that the above participant took part in a cycle of external quality assessment and achieved an acceptable level of performance (Cycle Average Absolute SDI ≤ 2) for the following parameters:

5

6 Cycle Average Absolute SDI

Albumin - Bromocresol Purple - Siemens/Dade Dimension RxL/Max/Xpand	0.50
Alkaline Phosphatase - Dade Dimension, AMP buffer - Siemens/Dade Dimension RxL/Max/Xpand	1.22
ALT (GPT) - Tris buffer with P5P - Siemens/Dade Dimension RxL/Max/Xpand	0.53
Amylase, Total - Dade Behring 2-chloro-pNPG3 - Siemens/Dade Dimension RxL/Max/Xpand	0.34
AST (GOT) - Tris buffer with P5P - Siemens/Dade Dimension RxL/Max/Xpand	0.55
Bicarbonate - Enzymatic - Siemens/Dade Dimension RxL/Max/Xpand	1.08
Bilirubin, Direct - Diazo with Sulphanilic Acid - Siemens/Dade Dimension RxL/Max/Xpand	0.19
Bilirubin, Total - Diazo with Sulphanilic Acid - Siemens/Dade Dimension RxL/Max/Xpand	0.26
Calcium - Cresolphthalein complexone - Siemens/Dade Dimension RxL/Max/Xpand	0.49
Chloride - ISE, indirect - Siemens/Dade Dimension RxL/Max/Xpand	0.70
Cholesterol - Dimension-Dade Behring reagents - Siemens/Dade Dimension RxL/Max/Xpand	0.54
CK, Total - CK-NAC (IFCC) - Siemens/Dade Dimension RxL/Max/Xpand	0.26
Creatinine - Alkaline picrate no deprot. - Siemens/Dade Dimension RxL/Max/Xpand	0.44
GGT - Gamma glut'3-carb'4-nitro (IFCC) - Siemens/Dade Dimension RxL/Max/Xpand	0.25
Glucose - Hexokinase - Siemens/Dade Dimension RxL/Max/Xpand	0.70

1	Full registration address	Your full registration address details.
2	Your lab reference number	Used to identify each lab.
3	Programme / cycle number	Programme and current, completed cycle number.
4	Date	Date End-of-Cycle report is issued.
5	Parameters	List of parameters including the assay details for which cycle absolute SDI is ≤ 2 .
6	Average Absolute SDI	Your Cycle Average Absolute SDI.

MONITORING EQA PERFORMANCE


Each EQA report should be evaluated and any poor performance investigated. A step by step approach should be adopted consisting of the following three steps:

1. Investigate the source of the problem

In order to identify the source of the problem, it is useful to be aware of the most common causes of poor EQA performance. Errors can occur at any stage of the testing process; however, EQA is most concerned with detecting analytical errors i.e. errors that occur during the analysis of the sample.

Most analytical errors can be easily divided into three main areas; clerical errors, systematic errors and random errors. Systematic errors result in inaccurate results that consistently show a positive or negative bias. Random errors, on the other hand, affect precision and result in fluctuations in either direction.

It may be possible that, after extensive investigations, the root cause of the poor performance cannot be established. Poor performance for a single sample could be attributed to random error. If poor performance has been noted for several samples, a systematic error is the most likely cause and the analytical process should be reviewed.

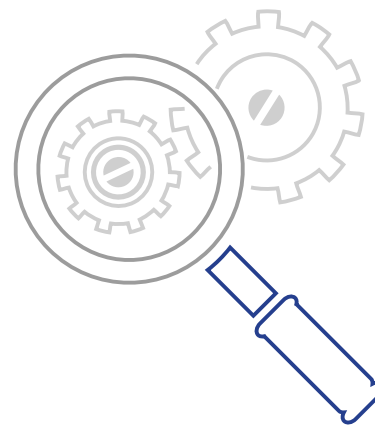

Clerical errors

- Transcription errors
- Incorrect units used
- Incorrect sample tested
- Incorrect method classification
- Calculation/conversion error

Systematic errors

- Sample/Reagent prep/handling
- Reagent/calibrator/standardisation change
- Instrument/reagent/calibrator fault
- Inexperienced operators
- Reagent deterioration
- Inappropriate method

Random errors

- Bubbles in reagent
- Bubbles in reagent/sample pipette
- Temperature fluctuations
- Poor pipetting technique
- Poor operator technique

The flowchart (page 29) is designed to help you investigate any apparent poor performance.

2. Implement corrective actions

Some errors can be readily recognised as simple clerical errors and easily corrected. If there is evidence of systematic or random error however more detailed corrective actions must be taken.

Systematic Error

In the event of a systematic error, the following suggested actions may help to resolve the problem:

- Perform instrument maintenance
- Recalibrate instrument
- Review reagent/sample storage
- Check pipettes
- Prepare fresh reagents & re-run sample
- Perform staff training

Random Error

If all possible causes have been excluded, a single unacceptable result is most likely due to random error. Re-run the sample; if the result of repeat analysis is acceptable then corrective action is not required. If the issue persists, investigate possible sources of systematic error.

3. Check the effectiveness of corrective actions

The effectiveness or impact of any corrective actions taken can be assessed by continuing to monitor analytical performance over time.

MONITORING EQA PERFORMANCE

A checklist similar to the one below is extremely useful when investigating poor EQA performance and may help you to determine the root cause of the problem and initiate corrective actions.

Laboratory:
 Cycle Number: Sample Number:
 Analysis Date: Analyte:
 Mean for Comparison: Lab Result: SDI: %Dev:

1. Specimen Handling

- a. Samples received in good condition Y N
- b. Samples stored/prepared appropriately Y N
- c. Integrity of the sample is acceptable Y N

2. Clerical

- a. Correct result entered Y N
- b. Correct use of decimal point and units Y N
- c. Calculations, if any, performed correctly (even if automated) Y N
- d. Conversion factors applied to results before submission Y N

3. Registration and Mean for Comparison

- a. Registered in the correct method/instrument group Y N
- b. Changed method or instrument without advising RIQAS Y N
- c. Peer Group changed due to the number of participants returning results e.g. from method to instrument Y N
- d. An obvious bias between method and instrument means (check histogram and stats sections) Y N

4. Internal Quality Control

- a. %Deviation of IQC (at similar conc to that of EQA) on sample analysis date acceptable Y N
- b. Shift in IQC in the periods just before and after EQA sample analysis Y N
- c. Trends in IQC in the periods before and after EQA sample analysis Y N
- d. Random IQC variation on sample analysis date Y N

- e. Error due to imprecision; check IQC in terms of %Deviation compared to deviation observed in EQA Y N
- f. IQC target correctly assigned Y N

5. Calibration

- a. Date of last calibration
- b. Calibration frequency acceptable Y N
- c. Last calibration acceptable Y N

6. Instrument

- a. Daily maintenance performed on date of sample analysis Y N
- b. Special maintenance performed prior to sample analysis Y N
- c. Instrument operated correctly Y N
- d. Operator fully trained Y N

7. Reagents

- a. Reagents prepared and stored correctly Y N
- b. Reagents within open vial stability Y N

8. EQA sample

- a. Initial value
- b. Re-run value
- c. Issue observed in previous EQA samples at a similar concentration (check %Deviation by concentration and Levey Jennings charts) Y N
- d. All parameters affected (to the same extent) - possible reconstitution error (check %Deviation on summary pages) Y N

Conclusion:


Remedial Action:

Lab Manager: Date:

Lab Director: Date:

MONITORING EQA PERFORMANCE

The flow chart below can be used to help identify a possible root cause for poor EQA performance.

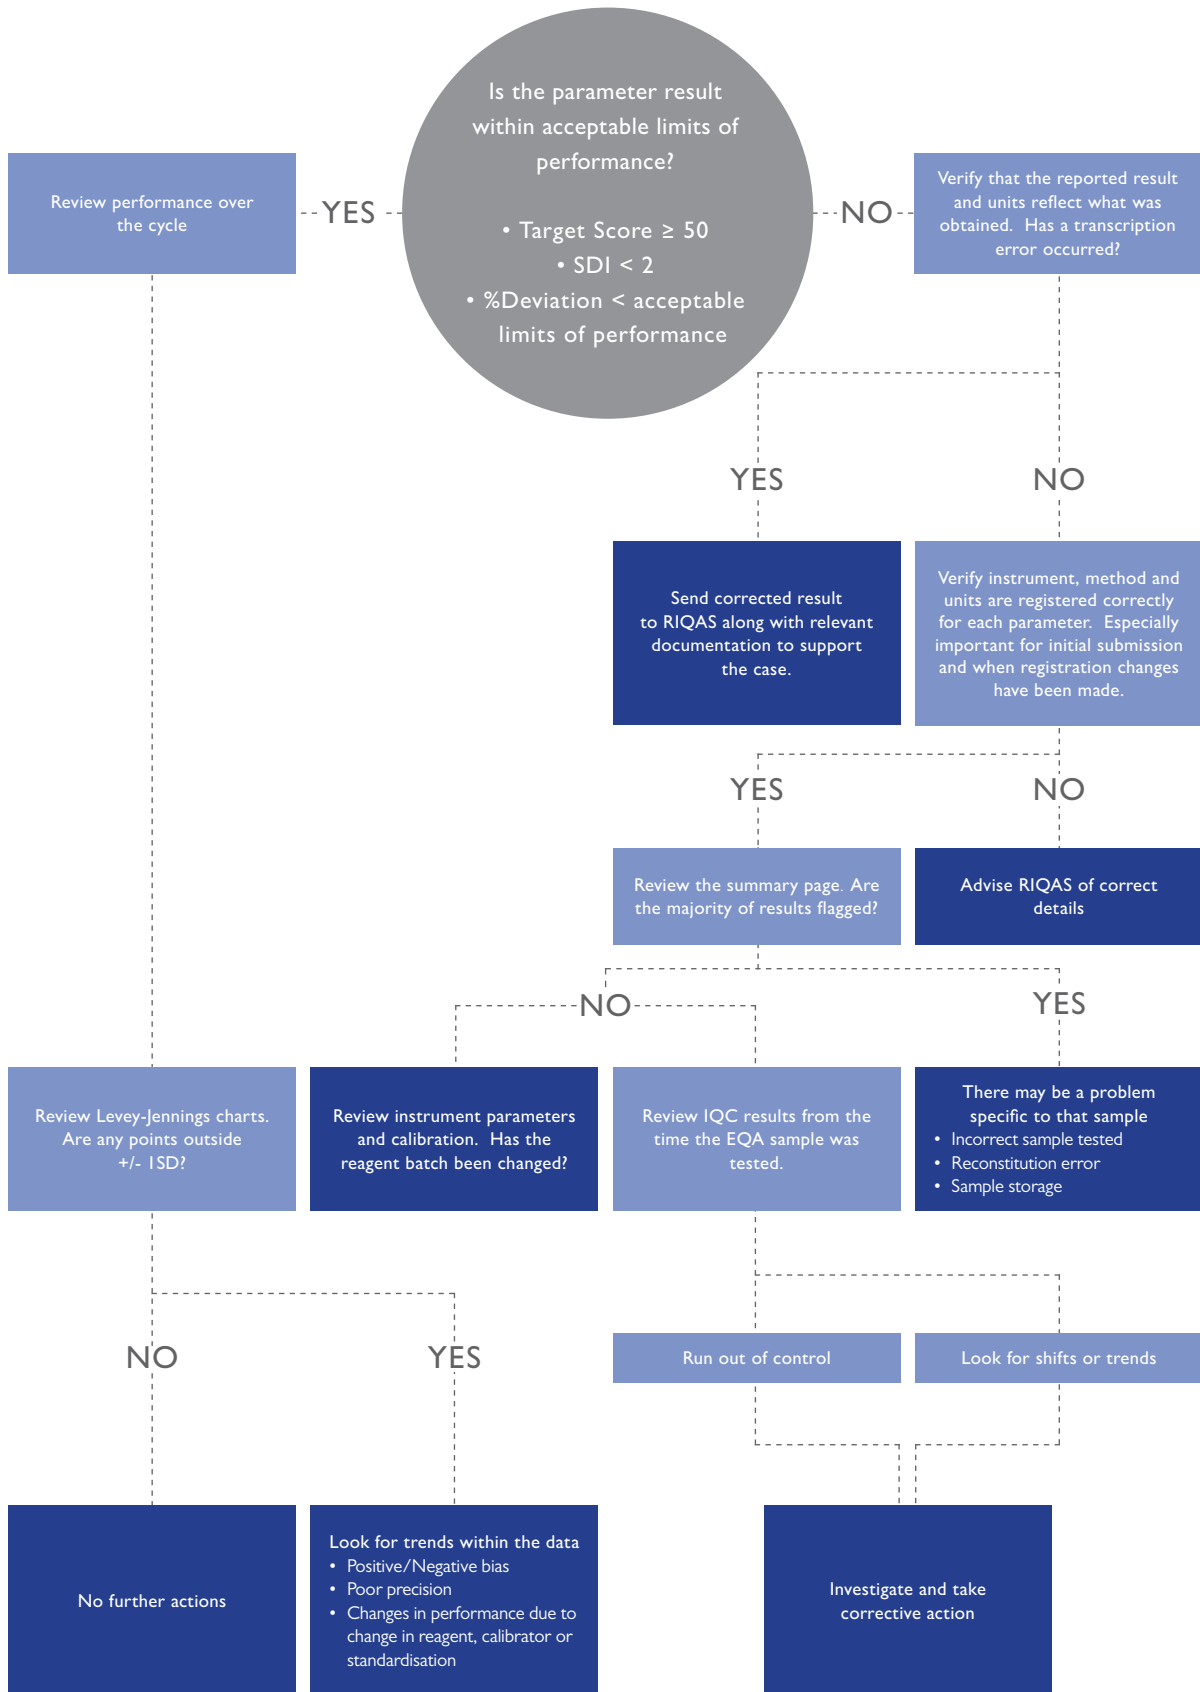

Ammonia/Ethanol Programme+ *With target scoring*

RQ9164 (2 ml)
2 Parameters
Samples every month, 1 x 12 month cycle, 12 month subscription

Ammonia Ethanol

Anti-TSH Receptor Programme+ *With target scoring*

RQ9174 (1 ml)
1 Parameter
Samples every month, 1 x 12 month cycle, 12 month subscription

Anti-TSH Receptor (TRAb)

Blood Gas Programme *With target scoring*

RQ9134 (1.8 ml) First registered instrument 10 Parameters Samples every month, 1 x 12 month cycle, 12 month subscription	RQ9134/A (1.8 ml) Subsequent instruments 10 Parameters
---	--

pCO ₂	CO ₂ (Total)*	K+	Lactate
pH	Ca ⁺⁺	Na+	
pO ₂	Cl ⁻	Glucose	

BNP Programme+ *With target scoring*

RQ9165 (1 ml)
1 Parameter
Samples every month, 1 x 12 month cycle, 12 month subscription

BNP

Cardiac Programme *With target scoring*

RQ9127/a (1 ml) 2 Parameters only (choose from 7) Samples every 2 weeks, 2 x 6 monthly cycles, 12 month subscription	RQ9127/b (1 ml) Full 7 Parameters
--	--------------------------------------

CK, Total	CK-MB (Mass)	Myoglobin	Troponin T
CK-MB (Activity)	Homocysteine	Troponin I	

Cerebrospinal Fluid Programme+ *With target scoring*


RQ9168 (3 ml)
7 Parameters
Samples every month, 1 x 12 month cycle, 12 month subscription

Albumin	Glucose	Lactate	Sodium
Chloride	IgG	Protein (Total)	

Coagulation Programme *With target scoring*

RQ9135/a (1 ml) 5 Selected parameters only (aPTT, PT, TT, Fibrinogen, Antithrombin III) Samples every month, 1 x 12 month cycle, 12 month subscription	RQ9135/b (1 ml) Full 17 Parameters
---	---------------------------------------

aPTT	Plasminogen	Factor VII	Factor XII
PT (including INR)	Protein C	Factor VIII	D-dimer*
TT	Protein S	Factor IX	
Fibrinogen	Factor II	Factor X	
Antithrombin III	Factor V	Factor XI	

 = Liquid ready-to-use samples

 = Lyophilised samples

PURPLE = The only parameters available on RQ9135/a

+ = Not accredited

* = Pilot study ongoing

RIQAS PROGRAMMES

CO-Oximetry Programme+

RQ9177 (1.2 ml) **RQ9177/A (1.2 ml)**
 First registered instrument Subsequent instruments
 7 Parameters 7 Parameters
 Samples every month, 1 x 12 month cycle, 12 month subscription

Carboxyhaemoglobin (COHb / HbCO) Methaemoglobin (MetHb) Oxygen Saturation (sO2 / Vol O2) Total Haemoglobin (tHb)
 Deoxyhaemoglobin (HHb) Oxygen Content (O2CT) Oxyhaemoglobin (O2Hb / HbO2)

CYFRA 21-I Programme+

RQ9175 (1 ml)
 1 Parameter
 Samples every month, 1 x 12 month cycle, 12 month subscription

CYFRA 21-I (Cytokeratin 19)

ESR Programme+

RQ9163 (4.5 ml)
 1 Parameter
 2 samples per quarterly distribution, 1 x 12 month cycle, 12 month subscription

ESR (Erythrocyte Sedimentation Rate)

General Clinical Chemistry Programme *With target scoring*

RQ9112/a (5 ml) **RQ9112/b (5 ml)** **RQ9112/c (5 ml)**
 10 Parameters only 17 Parameters only Full 52 Parameters
 Samples every 2 weeks, 2 x 6 monthly cycles, 12 month subscription, reference method values

ACE (Angiotensin Converting Enzyme)	Calcium	HBDH	PSA
Acid Phosphatase (Prostatic)	Calcium (Ionised)	HDL-Cholesterol	Sodium
Acid Phosphatase (Total)	Chloride	Iron	TIBC
Adjusted Calcium	Cholesterol	Lactate	T ₃ (Free)
Albumin	Cholinesterase	LD (LDH)	T ₃ (Total)
Alkaline Phosphatase	CK, Total (CPK)	Lipase	T ₄ (Free)
ALT (ALAT)	Copper	Lithium	T ₄ (Total)
Amylase (Pancreatic)	Creatinine	Magnesium	Triglycerides
Amylase (Total)	D-3-Hydroxybutyrate	NEFA	TSH
AST (ASAT)	EGFR	Non-HDL Cholesterol	UIBC
Bicarbonate	Fructosamine	Osmolality	Urea
Bile Acids	γGT	Phosphate (Inorganic)	Uric Acid
Bilirubin (Direct)	GLDH	Potassium	Zinc
Bilirubin (Total)	Glucose	Protein (Total)	

Glycated Haemoglobin Programme (HbA1c) *With target scoring*

RQ9129 (0.5ml)
 2 Parameters
 Samples every month, 1 x 12 month cycle, 12 month subscription

HbA1c Total Haemoglobin

Haematology Programme *With target scoring*

RQ9118 (2 ml)
 11 Parameters
 Samples every 2 weeks, 2 x 6 monthly cycles, 12 month subscription

Haematocrit (HCT)	Mean Cell Haemoglobin Concentration (MCHC)	Platelets (PLT)	Red Cell Distribution Width (RDW)
Haemoglobin (Hb)	Mean Cell Volume (MCV)	Plateletcrit (PCT)	Total White Blood Cell Count (WBC)
Mean Cell Haemoglobin (MCH)	Mean Platelet Volume (MPV)	Red Blood Cell Count (RBC)	

 = Liquid ready-to-use samples

 = Lyophilised samples

PURPLE = The only parameters available on RQ9135/a

+ = Not accredited

* = Pilot study ongoing

Human Urine Programme *With target scoring*

RQ9115 (10 ml)

25 Parameters

Samples every 2 weeks, 2 x 6 monthly cycles, 12 month subscription

ACR	Creatinine	Normetanephrine	Protein (Total)
Albumin/Microalbumin	Dopamine	Magnesium	Sodium
Amylase	Epinephrine	Osmolality	Urea
Calcium	Glucose	Oxalate	Uric Acid
Chloride	Metanephrine	Phosphate (Inorganic)	VMA
Copper	Norepinephrine	Potassium	5-HIAA
Cortisol			

Immunoassay Programme *With target scoring*

RQ9125/a (5 ml)

4 Parameters only (choose from 55)

Samples every two weeks, 2 x 6 monthly cycles, 12 month subscription (RQ9125/a, RQ9125/b, RQ9125/c)

Samples every month, 1 x 12 month cycle, 12 month subscription (RQ9130)

RQ9125/b (5 ml)

13 Parameters only (choose from 55)

RQ9125/c (5 ml)

Full 55 Parameters

RQ9130 (5 ml)

Full 55 Parameters

ACTH	DHEA Unconjugated	17-OH-Progesterone	T ₄ (Free)
AFP	Digoxin	Paracetamol	T ₄ (Total)
Aldosterone	Estriol Total*	Phenobarbital	Testosterone (Free)*
Amikacin	Ethosuximide*	Phenytoin	Testosterone (Total)
Androstenedione	Ferritin	Primidone*	Theophylline
β-2-Microglobulin	Folate	Progesterone	Thyroglobulin
CA125	FSH	Prolactin	Tobramycin*
CA15-3	Gentamicin	PSA (Free)	TSH
CA19-9	GH	PSA (Total)	Valproic Acid
Carbamazepine	hCG	PTH	Vancomycin
CEA	IgE	Salicylate	Vitamin B12
Cortisol	Insulin	SHBG	1-25-(OH) ₂ -Vitamin D*
C-Peptide	LH	T ₃ (Free)	25-OH-Vitamin D
DHEA-Sulphate	Oestradiol	T ₃ (Total)	

Immunoassay Speciality 1 Programme+ *With target scoring*

RQ9141 (2 ml)

10 Parameters

Samples every month, 1 x 12 month cycle, 12 month subscription

1-25-(OH) ₂ -Vitamin D*	Anti-TG	Osteocalcin	Insulin
25-OH-Vitamin D	Anti-TPO	Procalcitonin	
C-Peptide	IGF-I	PTH	

Immunoassay Speciality 2 Programme+ *With target scoring*

RQ9142 (1 ml)

5 Parameters

Samples every month, 1 x 12 month cycle, 12 month subscription

Calcitonin	Procalcitonin	Plasma Renin Activity	Renin (Direct Concentration)
Gastrin			

Immunosuppressant Programme+

RQ9159 (2 ml)

4 Parameters

Samples every month, 1 x 12 month cycle, 12 month subscription, reference method values

Ciclosporin	Everolimus	Sirolimus	Tacrolimus
-------------	------------	-----------	------------

Lipid Programme *With target scoring*

RQ9126/a (3 ml)

3 Parameters only (choose from 7)

Samples every 2 weeks, 2 x 6 monthly cycles, 12 month subscription

RQ9126/b (3 ml)

Full 7 Parameters

Apolipoprotein A1	Cholesterol (Total)	LDL-Cholesterol	Triglycerides
Apolipoprotein B	HDL-Cholesterol	Lipoprotein (a)	

 = Liquid ready-to-use samples

 = Lyophilised samples

PURPLE = The only parameters available on RQ9135/a

+ = Not accredited

* = Pilot study ongoing

RIQAS PROGRAMMES

Liquid Cardiac Programme *With target scoring*

RQ9136 (3 ml)
9 Parameters
Samples every month, 1 x 12 month cycle, 12 month subscription

CK-MB Mass	Homocysteine	Myoglobin	Troponin I
D-dimer	hsCRP	NT proBNP	Troponin T
Digoxin			

Maternal Screening Programme *With target scoring*

RQ9137 (1 ml)
6 Parameters
Samples every month, 1 x 12 month cycle, 12 month subscription

AFP	Total hCG	PAPP-A	Unconjugated Oestriol
free β-hCG	Inhibin A		

Serology (EBV) Programme+

RQ9153 (1 ml)
3 Parameters
3 samples per quarterly distribution, 1 x 12 month cycle, 12 month subscription, Quantitative and Qualitative results

Anti-EBV VCA IgG	Anti-EBNA IgG	Anti-EBV VCA IgM
------------------	---------------	------------------

Serology (HIV-Hepatitis) Programme+

RQ9151 (1.8 ml)
10 Parameters
5 samples per quarterly distribution, 1 x 12 month cycle, 12 month subscription, Quantitative and Qualitative results

Anti-HIV-1	Anti-HCV	Anti-HTLV-II	HBsAg
Anti-HIV-2	Anti-HBc	Anti-HTLV-I&2 Combined	
Anti-HIV-I&2 Combined	Anti-HTLV-I	Anti-CMV	

Serology (Syphilis) Programme+

RQ9154 (1 ml)
1 Parameter
3 samples per quarterly distribution, 1 x 12 month cycle, 12 month subscription, Quantitative and Qualitative results

Syphilis (Methods available include immunoassay RPR, VDRL and TPHA)

Serology (ToRCH) Programme+

RQ9152 (1 ml)
12 Parameters
5 samples per quarterly distribution, 1 x 12 month cycle, 12 month subscription, Quantitative and Qualitative results

Anti-Toxoplasma IgG	Anti-Rubella IgM	Anti-HSV1 IgG	Anti-HSV 1 IgM
Anti-Toxoplasma IgM	Anti-CMV IgG	Anti-HSV2 IgG	Anti-HSV 2 IgM
Anti-Rubella IgG	Anti-CMV IgM	Anti-HSV-I&2 IgG Combined	Anti-HSV I + 2 IgM Combined

Specific Proteins Programme *With target scoring*

RQ9114 (3 ml)
26 Parameters
Samples every 2 weeks, 2 x 6 monthly cycles, 12 month subscription

AFP	β-2-Microglobulin	IgA	Lambda Light Chain (Total)
Albumin	Ceruloplasmin	IgE	Prealbumin (Transthyretin)
α-1-Acid glycoprotein	Complement C ₃	IgG	Retinol Binding Protein
α-1-Antitrypsin	Complement C ₄	IgM	Rheumatoid Factor
α-2-Macroglobulin	C-Reactive Protein	Kappa Light Chain (Free)	Transferrin
Anti Streptolysin O	Ferritin	Kappa Light Chain (Total)	
Antithrombin III	Haptoglobin	Lambda Light Chain (Free)	

 = Liquid ready-to-use samples

 = Lyophilised samples

PURPLE = The only parameters available on RQ9135/a

+ = Not accredited

* = Pilot study ongoing

Sweat Testing Programme+

RQ9173 (2 ml)
2 Parameters
Samples every month, 1 x 12 month cycle, 12 month subscription

Chloride Conductivity

Therapeutic Drugs Programme *With target scoring*

RQ9111 (5 ml)
18 Parameters
Samples every 2 weeks, 2 x 6 monthly cycles, 12 month subscription, Weighed-in values

Amikacin	Ethosuximide	Phenobarbital	Tobramycin
Caffeine	Gentamicin	Phenytoin	Valproic Acid
Carbamazepine	Lithium	Primidone	Vancomycin
Ciclosporin	Methotrexate	Salicylic Acid	
Digoxin	Paracetamol (Acetaminophen)	Theophylline	

Trace Elements In Blood Programme+

RQ9172 (3 ml)
7 Parameters
Samples every month, 1 x 12 month cycle, 12 month subscription

Copper Lead Manganese Zinc
Iodine Magnesium Selenium

Trace Elements In Serum Programme+

RQ9170 (3 ml)
10 Parameters
Samples every month, 1 x 12 month cycle, 12 month subscription

Aluminium Copper Manganese Zinc
Chromium Iodine Nickel
Cobalt Lead Selenium

Trace Elements In Urine Programme+

RQ9171 (3 ml)
11 Parameters
Samples every month, 1 x 12 month cycle, 12 month subscription

Cadmium Copper Magnesium Nickel
Chromium Iodine Manganese Thallium
Cobalt Lead Molybdenum

Urinalysis Programme+ *With scoring*

RQ9138 (12 ml)
14 Parameters
Samples every 2 months, 1 x 12 month cycle, 12 month subscription

Albumin	Galactose	Leukocytes	Specific Gravity
Bilirubin	Glucose	Nitrite	Urobilinogen
Blood	hCG	pH	
Creatinine	Ketones	Protein	

Urine Toxicology Programme+

RQ9139 (5 ml)
20 Parameters
Samples every month, 1 x 12 month cycle, 12 month subscription

Benzoylcegonine	d-Methamphetamine	MDMA	Phenobarbital
Buprenorphine	EDDP	Methadone	Secobarbital
Cannabinoids (THC)	Ethanol	Nortriptyline	
Cotinine	Free Morphine	Norpropoxyphene	
Creatinine	Lorazepam	Oxazepam	
d-Amphetamine	LSD	Phencyclidine	

 = Liquid ready-to-use samples

 = Lyophilised samples

PURPLE = The only parameters available on RQ9135/a

+ = Not accredited

* = Pilot study ongoing

Whilst every attempt is made to ensure that information is accurate and up-to-date, some information is subject to change, please contact RIQAS for current details.

PARAMETER INDEX

+ = Not accredited

* = Pilot study ongoing

PURPLE = The only parameters available on RQ9135/a

		Ammonia / Ethanol +	Anti-TSH Receptor +	Blood Gas	BNP +	Cardiac	Cerebrospinal Fluid +	Coagulation	CO-Oximetry +	CYFRA 21-1 +	ESR +	General Clinical Chemistry	HbA1c	Haematology	Human Urine	Immunoassay	Immunoassay Speciality 1 +	Immunoassay Speciality 2 +
#	I-25-(OH) ₂ -Vitamin D*															X	X	
	17-OH-Progesterone																X	
	25-OH-Vitamin D															X	X	
	5-HIAA													X				
A	α-1-Acid Glycoprotein																	
	α-1-Antitrypsin																	
	α-2-Macroglobulin																	
	ACE (Angiotensin Converting Enzyme)											X						
	Acid Phosphatase (Prostatic)											X						
	Acid Phosphatase (Total)											X						
	ACR														X			
	ACTH																X	
	Adjusted Calcium*											X						
	AFP																X	
	Albumin						X					X			X			
	Aldosterone																X	
	Alkaline Phosphatase											X						
	ALT (ALAT)											X						
	Aluminium																	
	Amikacin																X	
	Ammonia		X															
	Amylase (Pancreatic)												X					
	Amylase (Total)											X			X			
	Androstenedione																X	
	Anti Streptolysin O (ASO)																	
	Anti-CMV																	
	Anti-CMV IgG																	
	Anti-CMV IgM																	
	Anti-EBNA IgG																	
	Anti-EBV VCA IgG																	
	Anti-EBV VCA IgM																	
	Anti-HBc																	
	Anti-HCV																	
	Anti-HIV-1																	
	Anti-HIV-1 & 2 Combined																	
	Anti-HIV-2																	
	Anti-HSV- 1 & 2 IgG Combined																	
	Anti-HSV- 1 & 2 IgM Combined																	
	Anti-HSV1 IgG																	
	Anti-HSV1 IgM																	
	Anti-HSV2 IgG																	

PARAMETER INDEX

Immunosuppressant +	Lipid	Liquid Cardiac	Maternal Screening	Serology (EBV) +	Serology (HIV / Hepatitis) +	Serology (Syphilis) +	Serology (ToRCH) +	Specific Proteins	Sweat Testing +	Therapeutic Drug	Trace Elements in Blood +	Trace Elements in Serum +	Trace Elements in Urine +	Urinalysis +	Urine Toxicology +			
																	I-25-(OH) ₂ -Vitamin D*	#
																	17-OH-Progesterone	
																	25-OH-Vitamin D	
																	5-HIAA	
								X									α-1-Acid Glycoprotein	A
								X									α-1-Antitrypsin	
								X									α-2-Macroglobulin	
																	ACE (Angiotensin Converting Enzyme)	
																	Acid Phosphatase (Prostatic)	
																	Acid Phosphatase (Total)	
																	ACR	
																	ACTH	
																	Adjusted Calcium*	
			X					X									AFP	
								X						X			Albumin	
																	Aldosterone	
																	Alkaline Phosphatase	
												X					ALT (ALAT)	
										X							Aluminium	
											X						Amikacin	
																	Ammonia	
																	Amylase (Pancreatic)	
																	Amylase (Total)	
																	Androstenedione	
								X									Anti Streptolysin O (ASO)	
					X												Anti-CMV	
						X											Anti-CMV IgG	
						X											Anti-CMV IgM	
				X													Anti-EBNA IgG	
				X													Anti-EBV VCA IgG	
				X													Anti-EBV VCA IgM	
					X												Anti-HBc	
					X												Anti-HCV	
					X												Anti-HIV-1	
					X												Anti-HIV-1 & 2 Combined	
					X												Anti-HIV-2	
						X											Anti-HSV- 1 & 2 IgG Combined	
						X											Anti-HSV- 1 & 2 IgM Combined	
						X											Anti-HSV1 IgG	
						X											Anti-HSV1 IgM	
						X											Anti-HSV2 IgG	

+ = Not accredited

* = Pilot study ongoing

PURPLE = The only parameters available on RQ9135/a

PARAMETER INDEX

+ = Not accredited

* = Pilot study ongoing

PURPLE = The only parameters available on RQ9135/a

		Ammonia / Ethanol +	Anti-TSH Receptor +	Blood Gas	BNP +	Cardiac	Cerebrospinal Fluid +	Coagulation	CO-Oximetry +	CYFRA 21-1 +	ESR +	General Clinical Chemistry	HbA1c	Haematology	Human Urine	Immunoassay	Immunoassay Speciality 1 +	Immunoassay Speciality 2 +
A	Anti-HSV2 IgM																	
	Anti-HTLV-1 & 2 Combined																	
	Anti-HTLV-I																	
	Anti-HTLV-II																	
	Anti-Rubella IgG																	
	Anti-Rubella IgM																	
	Anti-TG																	X
	Antithrombin III							X										
	Anti-Toxoplasma IgG																	
	Anti-Toxoplasma IgM																	
	Anti-TPO																	X
	Anti-TSH Receptor (TRAb)		X															
	Apolipoprotein AI																	
	Apolipoprotein B																	
	aPTT								X									
	AST (ASAT)												X					
B	β-2-Microglobulin																X	
	Benzoylcegonine																	
	Bicarbonate			X								X						
	Bile Acids											X						
	Bilirubin (Direct)											X						
	Bilirubin (Total)											X						
	Blood																	
	BNP				X													
	Buprenorphine																	
C	CA15-3																X	
	CA19-9																X	
	CA125																X	
	Cadmium																	
	Caffeine																	
	Calcitonin																	X
	Calcium											X			X			
	Calcium (Ionised)			X								X						
	Cannabinoids (THC)																	
	Carbamazepine																X	
	Carboxyhaemoglobin (COHb / HbCO)									X								
	CEA																X	
	Ceruloplasmin																	
	Chloride			X			X					X			X			
	Cholesterol (Total)											X						

PARAMETER INDEX

Immunosuppressant +	Lipid	Liquid Cardiac	Maternal Screening	Serology (EBV) +	Serology (HIV / Hepatitis) +	Serology (Syphilis) +	Serology (ToRCH) +	Specific Proteins	Sweat Testing +	Therapeutic Drug	Trace Elements in Blood +	Trace Elements in Serum +	Trace Elements in Urine +	Urinalysis +	Urine Toxicology +		
							X									Anti-HSV2 IgM	A
				X												Anti-HTLV-I & 2 Combined	
				X												Anti-HTLV-I	
				X												Anti-HTLV-II	
							X									Anti-Rubella IgG	
							X									Anti-Rubella IgM	
																Anti-TG	
								X								Antithrombin III	
							X									Anti-Toxoplasma IgG	
							X									Anti-Toxoplasma IgM	
																Anti-TPO	
																Anti-TSH Receptor (TRAb)	
	X															Apolipoprotein AI	
	X															Apolipoprotein B	
																aPTT	
																AST (ASAT)	
								X								β-2-Microglobulin	B
														X		Benzoylcegonine	
																Bicarbonate	
																Bile Acids	
																Bilirubin (Direct)	
														X		Bilirubin (Total)	
														X		Blood	
																BNP	
															X	Buprenorphine	
																CA15-3	
																CA19-9	C
																CA125	
													X			Cadmium	
										X						Caffeine	
																Calcitonin	
																Calcium	
																Calcium (Ionised)	
															X	Cannabinoids (THC)	
										X						Carbamazepine	
																Carboxyhaemoglobin (COHb / HbCO)	
																CEA	
								X								Ceruloplasmin	
									X							Chloride	
	X															Cholesterol (Total)	

+ = Not accredited

* = Pilot study ongoing

PURPLE = The only parameters available on RQ9135/a

PARAMETER INDEX

+ = Not accredited

* = Pilot study ongoing

PURPLE = The only parameters available on RQ9135/a

		Ammonia / Ethanol +	Anti-TSH Receptor +	Blood Gas	BNP +	Cardiac	Cerebrospinal Fluid +	Coagulation	CO-Oximetry +	CYFRA 21-I +	ESR +	General Clinical Chemistry	HbA1c	Haematology	Human Urine	Immunoassay	Immunoassay Speciality 1 +	Immunoassay Speciality 2 +	
C	Cholinesterase											X							
	Chromium																		
	Ciclosporin																		
	CK, Total					X						X							
	CK-MB (Activity)					X													
	CK-MB (Mass)					X													
	Cobalt																		
	Complement C ₃																		
	Complement C ₄																		
	Conductivity																		
	Copper											X			X				
	Cortisol														X	X			
	Cotinine																		
	C-Peptide															X	X		
	C-Reactive Protein (CRP)																		
	Creatinine											X			X				
CYFRA 21-I (Cytokeratin 19)									X										
D	D-3-Hydroxybutyrate										X								
	d-Amphetamine																		
	D-Dimer* ^Δ						X												
	Deoxyhaemoglobin (HHb)							X											
	DHEA Unconjugated															X			
	DHEA-Sulphate															X			
	Digoxin															X			
	d-Methamphetamine																		
	Dopamine														X				
E	EDDP											X							
	EGFR*											X							
	Epinephrine														X				
	ESR										X								
	Estriol Total*															X			
	Ethanol	X																	
	Ethosuximide* ^Δ															X			
	Everolimus																		
F	Factor II							X											
	Factor IX							X											
	Factor V							X											
	Factor VII							X											
	Factor VIII							X											
	Factor X							X											
	Factor XI							X											

^Δ Pilot status only in certain programmes. Please check pages 32 - 36 for more information.

PARAMETER INDEX

Immunosuppressant +	Lipid	Liquid Cardiac	Maternal Screening	Serology (EBV) +	Serology (HIV / Hepatitis) +	Serology (Syphilis) +	Serology (ToRCH) +	Specific Proteins	Sweat Testing +	Therapeutic Drug	Trace Elements in Blood +	Trace Elements in Serum +	Trace Elements in Urine +	Urinalysis +	Urine Toxicology +		
																Cholinesterase	C
												X	X			Chromium	
X										X						Ciclosporin	
																CK, Total	
																CK-MB (Activity)	
		X														CK-MB (Mass)	
												X	X			Cobalt	
								X								Complement C ₃	
								X								Complement C ₄	
									X							Conductivity	
										X	X	X				Copper	
															X	Cortisol	
																Cotinine	
								X								C-Peptide	
																C-Reactive Protein (CRP)	
													X	X		Creatinine	
																CYFRA 21-I (Cytokeratin 19)	
																D-3-Hydroxybutyrate	D
															X	d-Amphetamine	
		X														D-Dimer* ^Δ	
																Deoxyhaemoglobin (HHb)	
																DHEA Unconjugated	
																DHEA-Sulphate	
		X								X						Digoxin	
															X	d-Methamphetamine	
																Dopamine	
															X	EDDP	
																EGFR*	E
																Epinephrine	
																ESR	
																Estriol Total*	
															X	Ethanol	
										X						Ethosuximide* ^Δ	
X																Everolimus	F
																Factor II	
																Factor IX	
																Factor V	
																Factor VII	
																Factor VIII	
																Factor X	
																Factor XI	

+ = Not accredited

* = Pilot study ongoing

PURPLE = The only parameters available on RQ9135/a

^Δ Pilot status only in certain programmes. Please check pages 32 - 36 for more information.

PARAMETER INDEX

+ = Not accredited

* = Pilot study ongoing

PURPLE = The only parameters available on RQ9135/a

		Ammonia / Ethanol +	Anti-TSH Receptor +	Blood Gas	BNP +	Cardiac	Cerebrospinal Fluid +	Coagulation	CO-Oximetry +	CYFRA 21-1 +	ESR +	General Clinical Chemistry	HbA1c	Haematology	Human Urine	Immunoassay	Immunoassay Speciality 1 +	Immunoassay Speciality 2 +
F	Factor XII							X										
	Ferritin																X	
	Fibrinogen							X										
	Folate																X	
	Free Morphine																	
	free β-hCG																	
	Fructosamine											X						
	FSH																X	
G	γ-GT											X						
	Galactose																	
	Gastrin																	X
	Gentamicin																X	
	Growth Hormone (GH)																X	
	GLDH											X						
	Glucose			X			X					X			X			
H	Haematocrit (HCT)													X				
	Haemoglobin (Hb)													X				
	Total Haemoglobin (tHb)								X				X					
	Haptoglobin																	
	HbA1c												X					
	HBsAG																	
	HBDH											X						
	hCG																X	
	HDL-Cholesterol											X						
	Homocysteine					X												
	hsCRP																	
	I	IgA																
IgE																	X	
IGF-I																		X
IgG							X											
IgM																		
Inhibin A																		
Insulin																	X	X
Iodine																		
Iron												X						
K		Kappa Light Chain (Free)																
	Kappa Light Chain (Total)																	
	Ketones																	
L	Lactate			X			X					X						
	Lambda Light Chain (Free)																	

PARAMETER INDEX

Immunosuppressant +	Lipid	Liquid Cardiac	Maternal Screening	Serology (EBV) +	Serology (HIV / Hepatitis) +	Serology (Syphilis) +	Serology (ToRCH) +	Specific Proteins	Sweat Testing +	Therapeutic Drug	Trace Elements in Blood +	Trace Elements in Serum +	Trace Elements in Urine +	Urinalysis +	Urine Toxicology +		
								X								Factor XII	F
																Ferritin	
																Fibrinogen	
																Folate	
			X												X	Free Morphine	G
																free β-hCG	
																Fructosamine	
																FSH	
																γ-GT	H
														X		Galactose	
										X						Gastrin	
																Gentamicin	
																Growth Hormone (GH)	I
																GLDH	
														X		Glucose	
																Haematocrit (HCT)	
																Haemoglobin (Hb)	K
																Total Haemoglobin (tHb)	
								X								Haptoglobin	
					X											HbA1c	
																HBsAG	L
																HBDH	
	X													X		hCG	
		X														HDL-Cholesterol	
			X													Homocysteine	I
																hsCRP	
								X								IgA	
								X								IgE	
																IGF- I	K
								X								IgG	
								X								IgM	
			X													Inhibin A	
																Insulin	L
											X	X	X			Iodine	
																Iron	
								X								Kappa Light Chain (Free)	
								X								Kappa Light Chain (Total)	K
														X		Ketones	
																Lactate	L
								X								Lambda Light Chain (Free)	

+ = Not accredited

* = Pilot study ongoing

PURPLE = The only parameters available on RQ9135/a

PARAMETER INDEX

+ = Not accredited

* = Pilot study ongoing

PURPLE = The only parameters available on RQ9135/a

		Ammonia / Ethanol +	Anti-TSH Receptor +	Blood Gas	BNP +	Cardiac	Cerebrospinal Fluid +	Coagulation	CO-Oximetry +	CYFRA 21-I +	ESR +	General Clinical Chemistry	HbA1c	Haematology	Human Urine	Immunoassay	Immunoassay Speciality 1 +	Immunoassay Speciality 2 +
L	Lambda Light Chain (Total)																	
	LD (LDH)											X						
	LDL-Cholesterol																	
	Lead																	
	Leukocytes																	
	Lipase											X						
	Lipoprotein (a)																	
	Lithium											X						
	Lorazepam																	
	LSD																	
	Luteinising Hormone (LH)																X	
M	Magnesium											X			X			
	Manganese																	
	MDMA																	
	Mean Cell Haemoglobin (MCH)													X				
	Mean Cell Haemoglobin Concentration (MCHC)													X				
	Mean Cell Volume (MCV)													X				
	Mean Platelet Volume (MPV)													X				
	Metanephrine															X		
	Methadone																	
	Methaemoglobin (MetHb)								X									
	Methotrexate																	
	Molybdenum																	
	Myoglobin					X												
	N	NEFA											X					
Nickel																		
Nitrite																		
Non-HDL Cholesterol*												X						
Norepinephrine															X			
Normetanephrine															X			
Norpropoxyphene																		
Nortriptyline																		
NTproBNP																		
O	Oestradiol															X		
	Osmolality											X			X			
	Osteocalcin																X	
	Oxalate														X			
	Oxazepam																	
	Oxygen Content (O2CT)								X									
	Oxygen Saturation (sO2 / Vol O2)								X									
	Oxyhaemoglobin (O2Hb / HbO2)								X									

PARAMETER INDEX

Immunosuppressant +	Lipid	Liquid Cardiac	Maternal Screening	Serology (EBV) +	Serology (HIV / Hepatitis) +	Serology (Syphilis) +	Serology (ToRCH) +	Specific Proteins	Sweat Testing +	Therapeutic Drug	Trace Elements in Blood +	Trace Elements in Serum +	Trace Elements in Urine +	Urinalysis +	Urine Toxicology +		
								X								Lambda Light Chain (Total)	L
																LD (LDH)	
	X															LDL-Cholesterol	
											X	X	X			Lead	
														X		Leukocytes	
																Lipase	
	X															Lipoprotein (a)	
										X						Lithium	
															X	Lorazepam	
															X	LSD	
																Luteinising Hormone (LH)	
											X		X			Magnesium	M
											X	X	X			Manganese	
														X		MDMA	
																Mean Cell Haemoglobin (MCH)	
																Mean Cell Haemoglobin Concentration (MCHC)	
																Mean Cell Volume (MCV)	
																Mean Platelet Volume (MPV)	
																Metanephrine	
															X	Methodone	
																Methaemoglobin (MetHb)	
										X						Methotrexate	
													X			Molybdenum	
		X														Myoglobin	
																NEFA	N
												X	X			Nickel	
														X		Nitrite	
																Non-HDL Cholesterol*	
																Norepinephrine	
																Normetanephrine	
															X	Norpropoxyphene	
															X	Nortriptyline	
		X														NTproBNP	
																Oestradiol	O
																Osmolality	
																Osteocalcin	
																Oxalate	
															X	Oxazepam	
																Oxygen Content (O2CT)	
																Oxygen Saturation (sO2 / Vol O2)	
																Oxyhaemoglobin (O2Hb / HbO2)	

+ = Not accredited

* = Pilot study ongoing

PURPLE = The only parameters available on RQ9135/a

PARAMETER INDEX

+ = Not accredited

* = Pilot study ongoing

PURPLE = The only parameters available on RQ9135/a

		Ammonia / Ethanol +	Anti-TSH Receptor +	Blood Gas	BNP +	Cardiac	Cerebrospinal Fluid +	Coagulation	CO-Oximetry +	CYFRA 21-I +	ESR +	General Clinical Chemistry	HbA1c	Haematology	Human Urine	Immunoassay	Immunoassay Speciality 1 +	Immunoassay Speciality 2 +
P	PAPP-A																	
	Paracetamol (Acetaminophen)																X	
	pCO ₂			X														
	pH			X														
	Phencyclidine																	
	Phenobarbital																X	
	Phenytoin																X	
	Phosphate (Inorganic)											X				X		
	Plasma Renin Activity																	X
	Plasminogen								X									
	Plateletcrit (PCT)													X				
	Platelets (PLT)													X				
	pO ₂			X														
	Potassium			X								X				X		
	Prealbumin (Transthyretin)																	
	Primidone* ^Δ																X	
	Procalcitonin																	X
	Progesterone																X	
	Prolactin																X	
	Protein (Total)							X				X				X		
	Protein C								X									
	Protein S								X									
	PSA (Free)																X	
	PSA (Total)											X					X	
	PT (Including INR)								X									
	PTH																X	X
R	Red Blood Cell Count (RBC)													X				
	Red Cell Distribution Width (RDW)													X				
	Renin (Direct Concentration)																	
	Retinol Binding Protein																	
	Rheumatoid Factor																	
S	Salicylic Acid															X		
	Secobarbital																	
	Selenium																	
	SHBG															X		
	Sirolimus																	
	Sodium			X			X					X			X			
	Specific Gravity																	
	Syphilis																	
T	T ₃ (Free)										X					X		

^Δ Pilot status only in certain programmes. Please check pages 32 - 36 for more information.

PARAMETER INDEX

Immunosuppressant +	Lipid	Liquid Cardiac	Maternal Screening	Serology (EBV) +	Serology (HIV / Hepatitis) +	Serology (Syphilis) +	Serology (ToRCH) +	Specific Proteins	Sweat Testing +	Therapeutic Drug	Trace Elements in Blood +	Trace Elements in Serum +	Trace Elements in Urine +	Urinalysis +	Urine Toxicology +		
			X													PAPP-A	P
										X						Paracetamol (Acetaminophen)	
																pCO ₂	
														X		pH	
															X	Phencyclidine	
										X					X	Phenobarbital	
										X						Phenytoin	
																Phosphate (Inorganic)	
																Plasma Renin Activity	
																Plasminogen	
																Plateletcrit (PCT)	
																Platelets (PLT)	
																pO ₂	
																Potassium	
								X								Prealbumin (Transthyretin)	
										X						Primidone* ^Δ	
																Procalcitonin	
																Progesterone	
																Prolactin	
														X		Protein (Total)	
																Protein C	
																Protein S	
																PSA (Free)	
																PSA (Total)	
																PT (Including INR)	
																PTH	
																Red Blood Cell Count (RBC)	R
																Red Cell Distribution Width (RDW)	
																Renin (Direct Concentration)	
								X								Retinol Binding Protein	
								X								Rheumatoid Factor	
										X						Salicylic Acid	S
															X	Secobarbital	
											X	X				Selenium	
																SHBG	
X																Sirolimus	
																Sodium	
														X		Specific Gravity	
						X										Syphilis	
																T ₃ (Free)	T

+ = Not accredited

* = Pilot study ongoing

PURPLE = The only parameters available on RQ9135/a

^Δ Pilot status only in certain programmes. Please check pages 32 - 36 for more information.

PARAMETER INDEX

+ = Not accredited

* = Pilot study ongoing

PURPLE = The only parameters available on RQ9135/a

		Ammonia / Ethanol +	Anti-TSH Receptor +	Blood Gas	BNP +	Cardiac	Cerebrospinal Fluid +	Coagulation	CO-Oximetry +	CYFRA 21-1 +	ESR +	General Clinical Chemistry	HbA1c	Haematology	Human Urine	Immunoassay	Immunoassay Speciality 1 +	Immunoassay Speciality 2 +
T	T ₃ (Total)											X				X		
	T ₄ (Free)											X				X		
	T ₄ (Total)											X				X		
	Tacrolimus																	
	Testosterone (Free)*																X	
	Testosterone (Total)																X	
	Thallium																	
	Theophylline																X	
	Thyroglobulin																X	
	TIBC											X						
	Tobramycin* ^Δ																X	
	Total hCG																	
	Transferrin																	
	Triglycerides												X					
	Troponin I						X											
	Troponin T						X											
	TSH											X					X	
	TT								X									
U	UIBC											X						
	Unconjugated Oestriol																	
	Urea											X			X			
	Uric Acid											X			X			
	Urobilinogen																	
V	Valproic Acid																X	
	Vancomycin																X	
	Vitamin B12																X	
	VMA														X			
W	Total White Blood Cell Count (WBC)												X					
Z	Zinc											X						

^Δ Pilot status only in certain programmes. Please check pages 32 - 36 for more information.

PARAMETER INDEX

Immunosuppressant +	Lipid	Liquid Cardiac	Maternal Screening	Serology (EBV) +	Serology (HIV / Hepatitis) +	Serology (Syphilis) +	Serology (ToRCH) +	Specific Proteins	Sweat Testing +	Therapeutic Drug	Trace Elements in Blood +	Trace Elements in Serum +	Trace Elements in Urine +	Urinalysis +	Urine Toxicology +		
																T ₃ (Total)	T
																T ₄ (Free)	
																T ₄ (Total)	
X																Tacrolimus	
																Testosterone (Free)*	
																Testosterone (Total)	
													X			Thallium	
										X						Theophylline	
																Thyroglobulin	
																TIBC	
										X						Tobramycin* ^Δ	
			X													Total hCG	
								X								Transferrin	
	X															Triglycerides	
		X														Troponin I	
		X														Troponin T	
																TSH	
																TT	
																UIBC	U
			X													Unconjugated Oestriol	
																Urea	
																Uric Acid	
													X			Urobilinogen	
										X						Valproic Acid	V
										X						Vancomycin	
																Vitamin B12	
																VMA	
																Total White Blood Cell Count (WBC)	W
											X	X				Zinc	Z

+ = Not accredited

* = Pilot study ongoing

PURPLE = The only parameters available on RQ9135/a

^Δ Pilot status only in certain programmes. Please check pages 32 - 36 for more information.

RELATED PRODUCTS

ACUSERA True Third Party Quality Controls

As a world leading manufacturer of multi-analyte true third party controls, thousands of laboratories rely on Randox to accurately assess test system performance and ultimately empower them with the confidence required to release patient test results. With more than 400 analytes available, the number of individual controls required to cover your test menu is significantly reduced while simultaneously reducing costs, time and storage space. A choice of formats is available, including liquid or lyophilised, which ensures flexibility and suitability for laboratories of all sizes and budgets. Many features of the Acusera range can help you to meet ISO 15189:2012 requirements:

- Designed to react to the test system in the same manner as a patient sample, helping to reduce inconvenient shifts in QC results when reagent batch is changed and ultimately providing a true indication of laboratory performance.
- The presence of analytes at key decision levels ensures accurate instrument performance and eliminates the need for additional low/high controls at extra expense.
- Manufactured independently from any instrument, the Acusera range delivers unbiased performance assessment with any instrument or method, while eliminating the need for multiple instrument specific controls.

Product Portfolio

Antioxidants | Blood Gas | Cardiac Markers | Routine Chemistry | Coagulation | Haematology | Diabetes | Immunoassay
Immunology | Infectious Diseases (Serology) | Lipids | POCT | Therapeutic Drugs | Toxicology | Urine Chemistry



Uniquely combining more than 100 analytes conveniently in a single control, laboratories can significantly reduce costs and consolidate without compromising on quality. As true third party controls, unbiased performance assessment with any instrument or method is guaranteed.


ACUSERA 24•7 Interlaboratory Data Management

Designed for use with the Acusera range of third party controls, the Acusera 24•7 software helps laboratories monitor and interpret their QC data. Access to an impressive range of features, including interactive charts, the automatic calculation of Measurement Uncertainty & Sigma Metrics and live peer group data generated from our extensive database of laboratory participants, ensures Acusera 24•7 is the most comprehensive package available.

- Advanced statistical analysis with automatic calculation of performance metrics including; Sigma, UM, TE & %Bias.
- Instantly discover how you compare to your peers with peer group statistics updated live in real-time reducing time and money spent troubleshooting.
- Interactive charts allowing you to add events and multiple data sets for quick and easy performance monitoring.
- Automated data import with bi-directional connection to LIMS (eliminating manual data entry).

Software Features

Dashboard | Result History | Interactive Levey-Jennings Charts | Interactive Histogram Charts
 Performance Summary Charts | Statistical Analysis Report | Statistical Metrics Report | Audit Trail Report
 Uncertainty of Measurement Report | Exception Report | Peer Group Statistics | Acusera Advisor

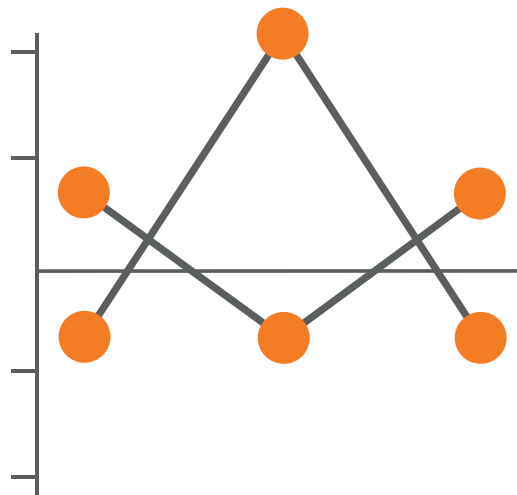

 'The laboratory shall have a procedure to prevent the release of patient results in the event of quality control failure. When the quality controls rules are violated and indicate that examination results are likely to contain significant errors the results shall be rejected... Quality Control data shall be reviewed at regular intervals to detect trends in examination performance.'

RANDOX - A GLOBAL DIAGNOSTIC SOLUTIONS PROVIDER

Randox has been supplying laboratories worldwide with revolutionary diagnostic solutions for over 35 years. Our experience and expertise allow us to create a leading product portfolio of high quality diagnostic tools which offer reliable and rapid diagnosis. We believe that by providing laboratories with the right tools, we can improve healthcare worldwide.



RX SERIES

Renowned for quality and reliability, the RX series combines robust hardware and intuitive software with the world leading RX series test menu comprising an extensive range of high quality reagents including routine chemistries, specific proteins, lipids, therapeutic drugs, drugs of abuse, antioxidants and diabetes testing. The RX series offers excellence in patient care delivering unrivalled precision and accuracy for results you can trust, guaranteeing real cost savings through consolidation of routine and specialised tests onto one single platform.



REAGENTS

Randox offers an extensive range of third-party diagnostic reagents which are internationally recognised as being of the highest quality; producing accurate and precise results. At Randox, we re-invest significantly in R&D to ensure we meet the ever-changing needs of the laboratory. Consequently, Randox offer a range of novel and superior performance assays, including: sdLDL-C, Lipoprotein (a), H-FABP, Adiponectin, Copper and Zinc. Applications are available detailing instrument-specific settings for the convenient use of Randox Reagents on numerous clinical chemistry analysers.



EVIDENCE SERIES

In 2002, Randox invented the world's first, Biochip Array Technology, offering highly specific tests, coupled to the highly sensitive chemiluminescent detection, providing quantitative results instantly changing the landscape of diagnostic testing forever. The Randox Evidence Series of multi-analyte immunoanalysers provide an unrivalled increase in patient information per sample offering diagnostic, prognostic and predictive solutions across a variety of disease areas with a highly advanced clinical and toxicology immunoassay test menu including cardiac, diabetes, drugs of abuse, metabolic and renal markers.

Contact us for more information on any of our products and services:

HEADQUARTERS

Randox Laboratories Ltd, 55 Diamond Road, Crumlin, County Antrim, BT29 4QY, United Kingdom

☎ +44 (0) 28 9445 4399 ✉ marketing@randox.com 🌐 riqas.com

INTERNATIONAL OFFICES



AUSTRALIA

Randox (Australia) Pty Ltd.
Tel: +61 (0) 2 9615 4640



BRAZIL

Randox Brasil Ltda.
Tel: +55 11 5181-2024



CHINA

Randox Laboratories Ltd.
Tel: +86 021 6288 6240



CZECH REPUBLIC

Randox Laboratories S.R.O.
Tel: +420 2 1115 1661



FRANCE

Laboratoires Randox
Tel: +33 (0) 130 18 96 80



GERMANY

Randox Laboratories GmbH
Tel: +49 (0) 215 1937 0611



HONG KONG

Randox Laboratories Hong Kong Limited
Tel: +852 3595 0515



ITALY

Randox Laboratories Ltd.
Tel: +39 06 9896 8954



INDIA

Randox Laboratories India Pvt Ltd.
Tel: +91 80 2802 5000



POLAND

Randox Laboratories Polska Sp. z o.o.
Tel: +48 22 862 1080



PORTUGAL

Irandox Laboratorios Quimica Analitica Ltda
Tel: +351 22 589 8320



PUERTO RICO

Clinical Diagnostics of Puerto Rico, LLC
Tel: +1 787 701 7000



REPUBLIC OF IRELAND

Randox Teoranta
Tel: +353 7495 22600



SLOVAKIA

Randox S.R.O.
Tel: +421 2 6381 3324



SOUTH AFRICA

Randox Laboratories SA (Pty) Ltd.
Tel: +27 (0) 11 312 3590



SOUTH KOREA

Randox Korea
Tel: +82 (0) 31 478 3121



SPAIN

Laboratorios Randox S.L.
Tel: +34 93 475 09 64



SWITZERLAND

Randox Laboratories Ltd. (Switzerland)
Tel: +41 41 810 48 89



UAE

Randox Medical Equipments Trading LLC
Tel: +971 55 474 9075



USA

Randox Laboratories-US, Ltd.
Tel: +1 304 728 2890




VIETNAM

Randox Laboratories Ltd. Vietnam
Tel: +84 (0) 8 391 1 0904

For technical support contact:

mail@riqas.com

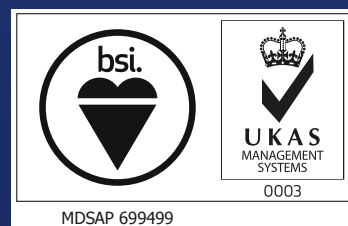

LT033 SEP19